



PARALLEL IMAGING COMPATIBLE
BIRDCAGE RESONATOR
10/723,428
MR/02-003

Replacement Sheet

1/25

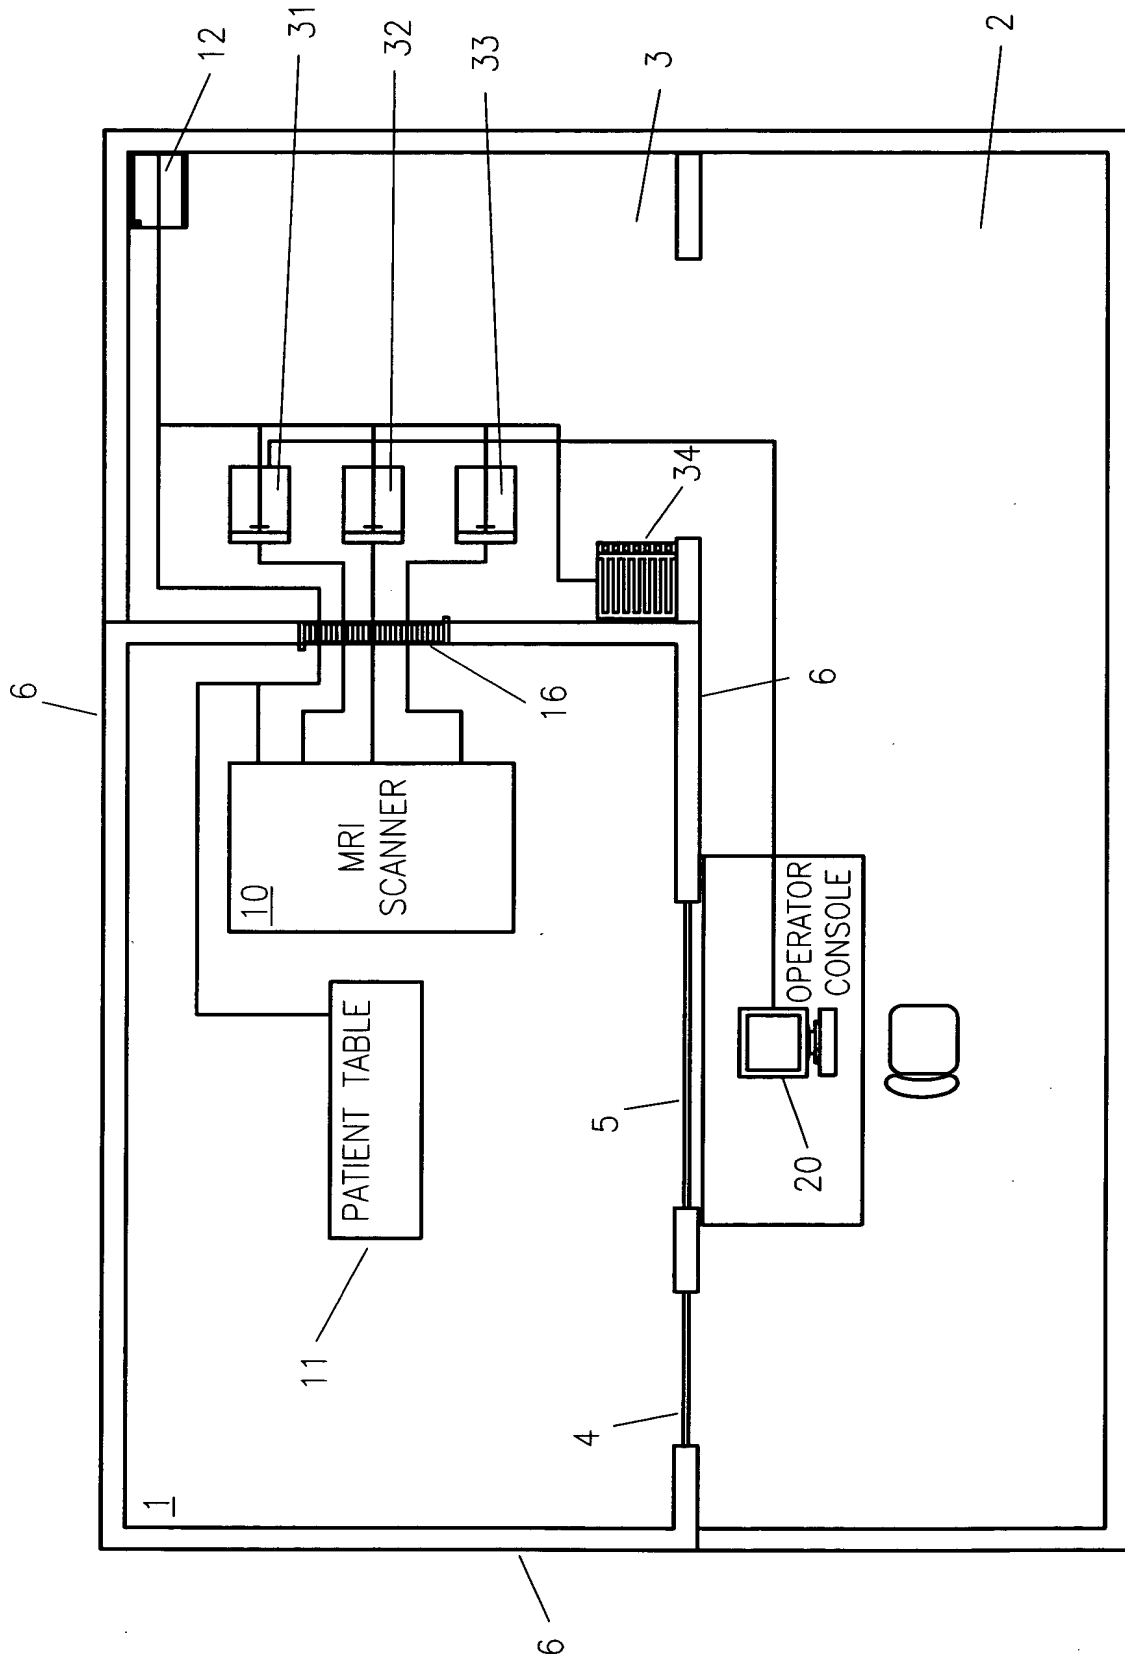


FIG. 1A

2/25

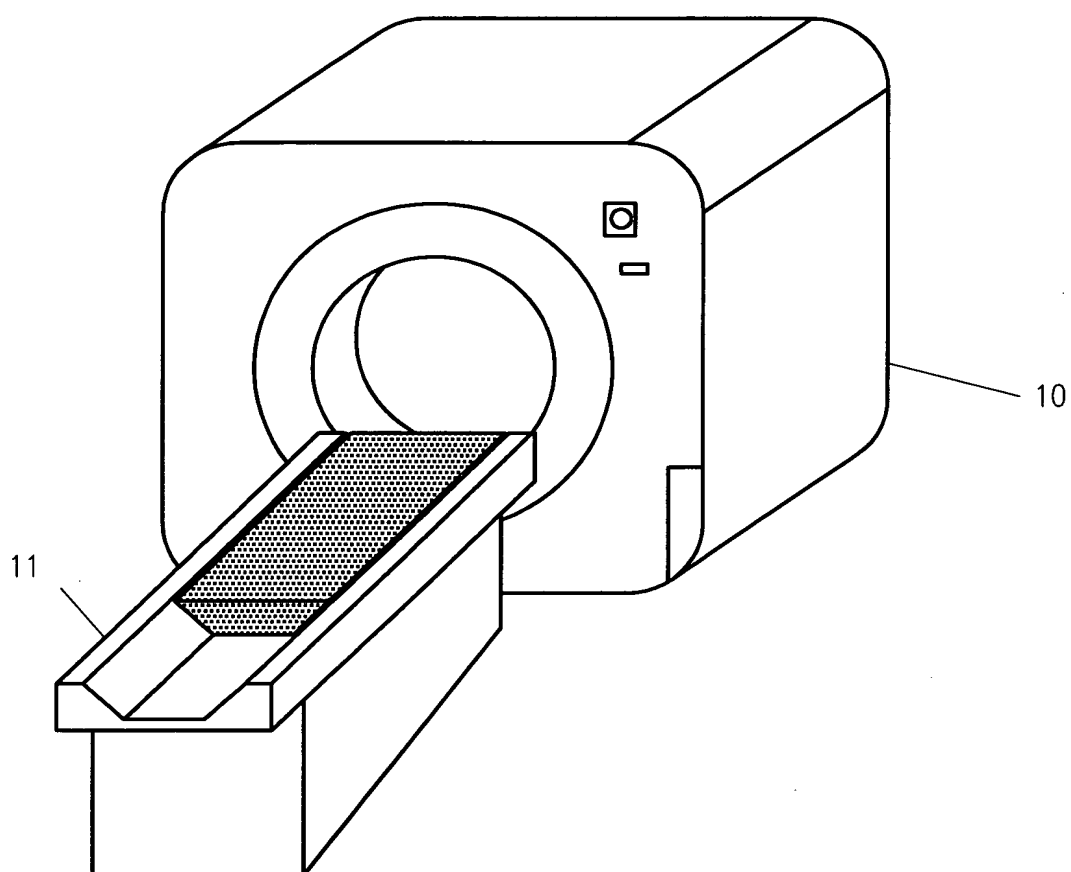


FIG. 1B

3/25


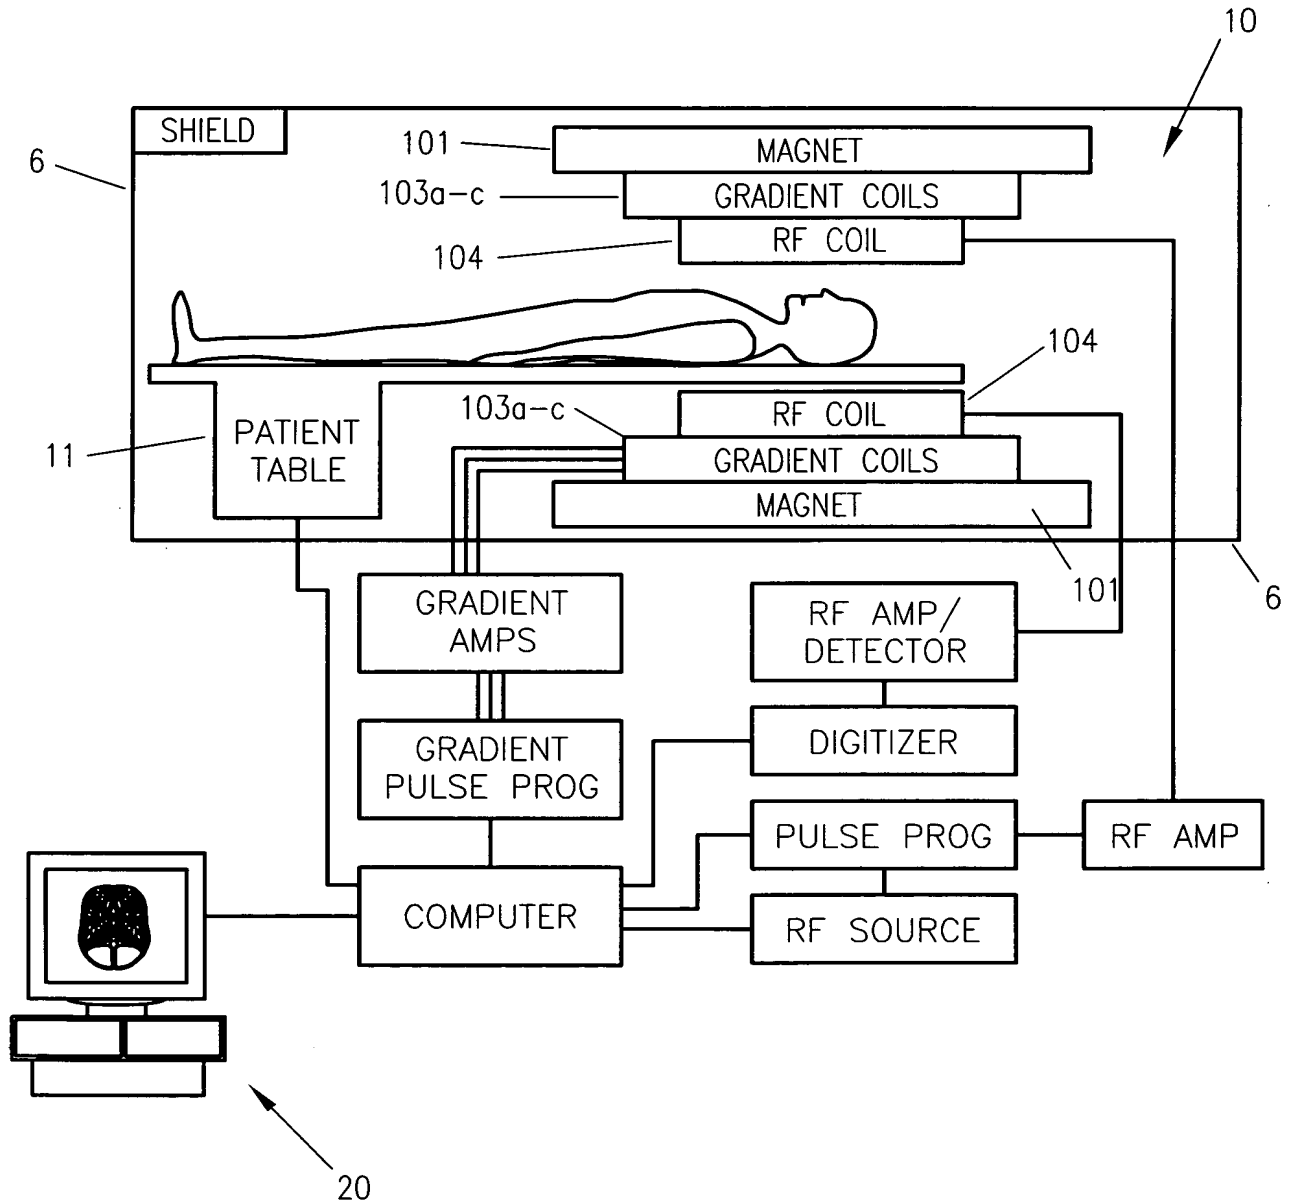



FIG. 1C

4/25

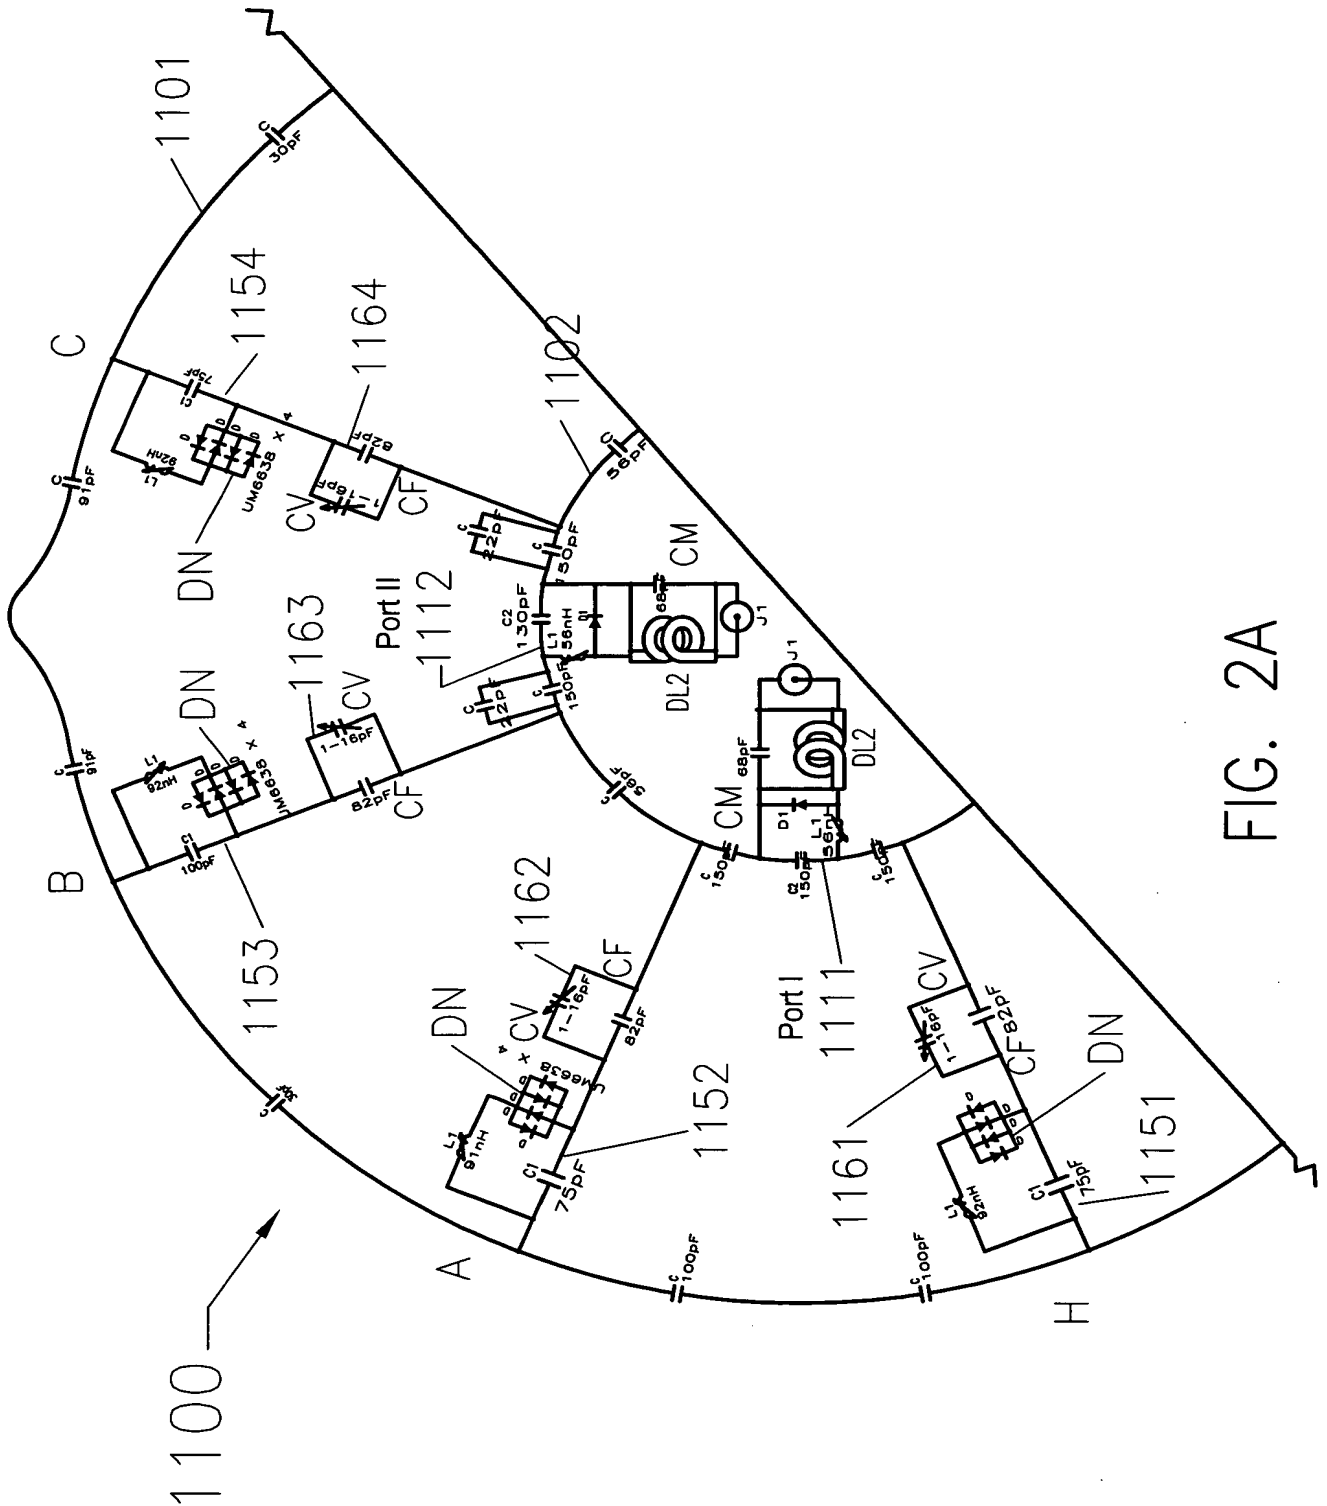

5/25

FIG. 2B

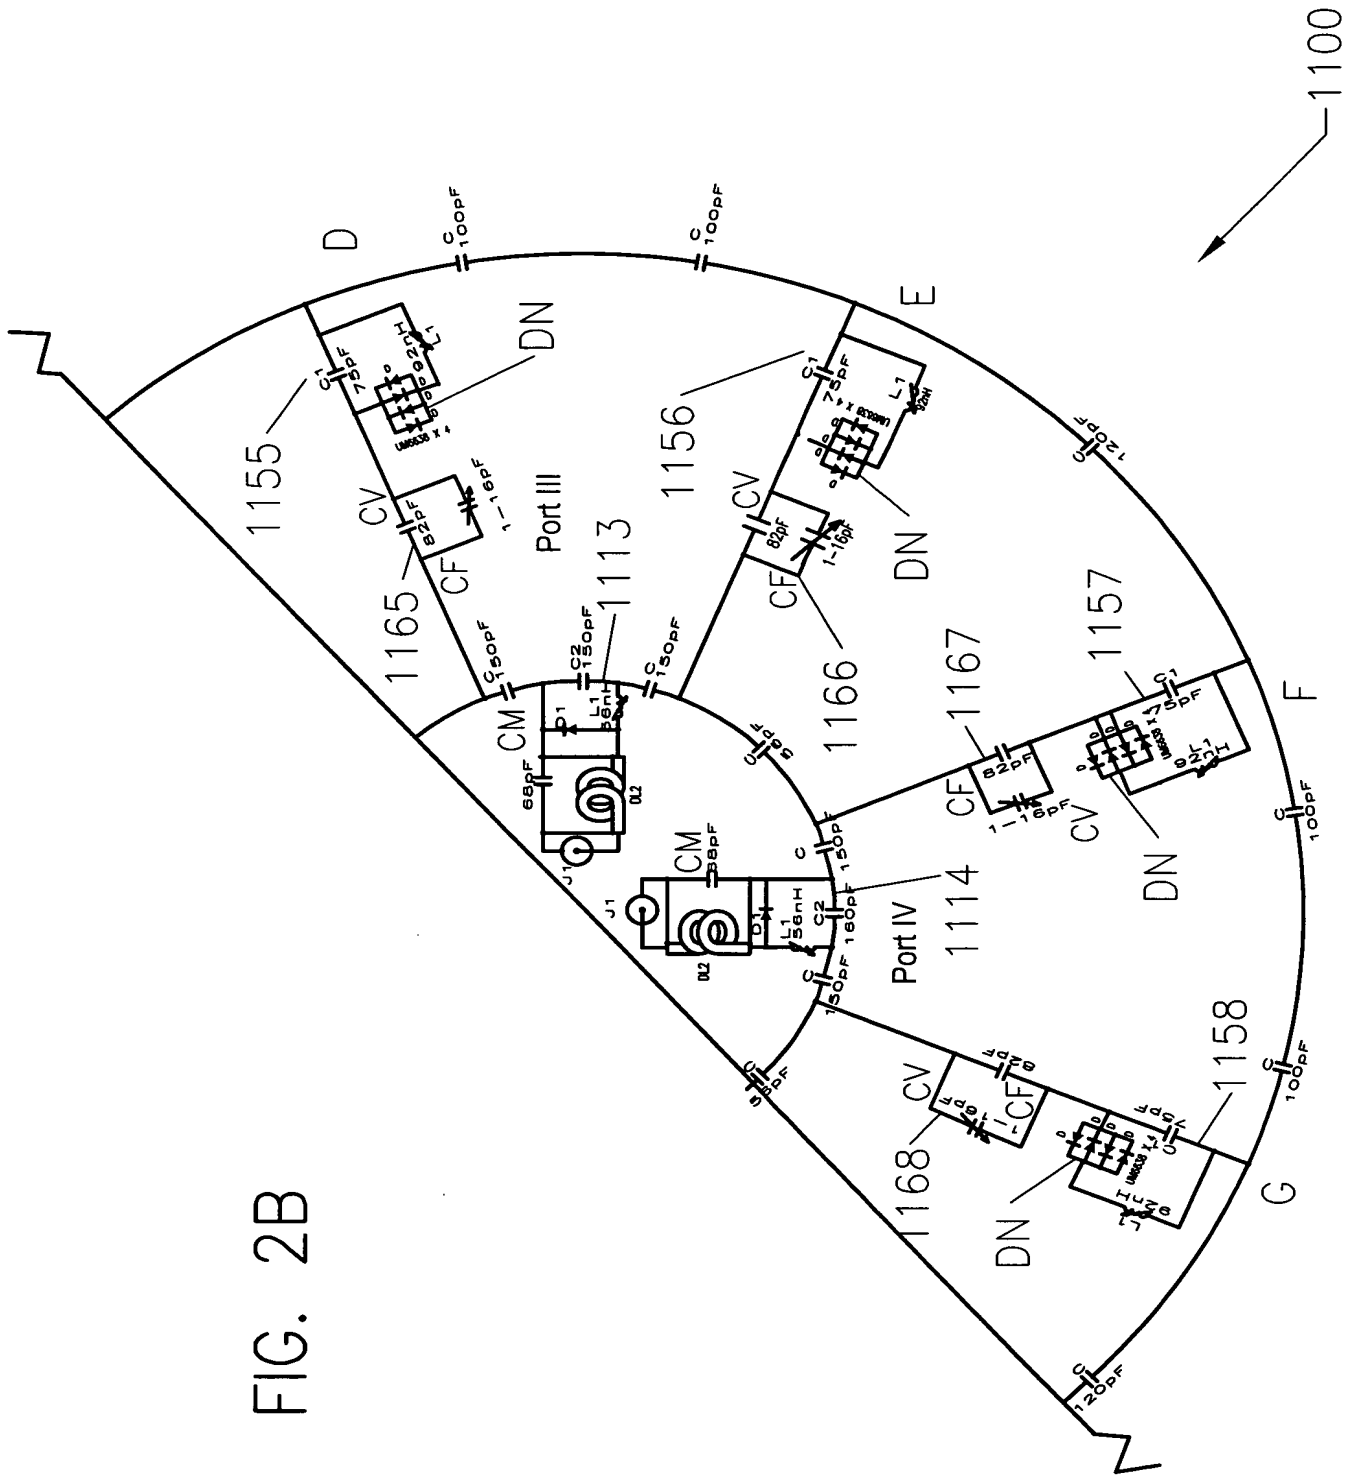

6/25

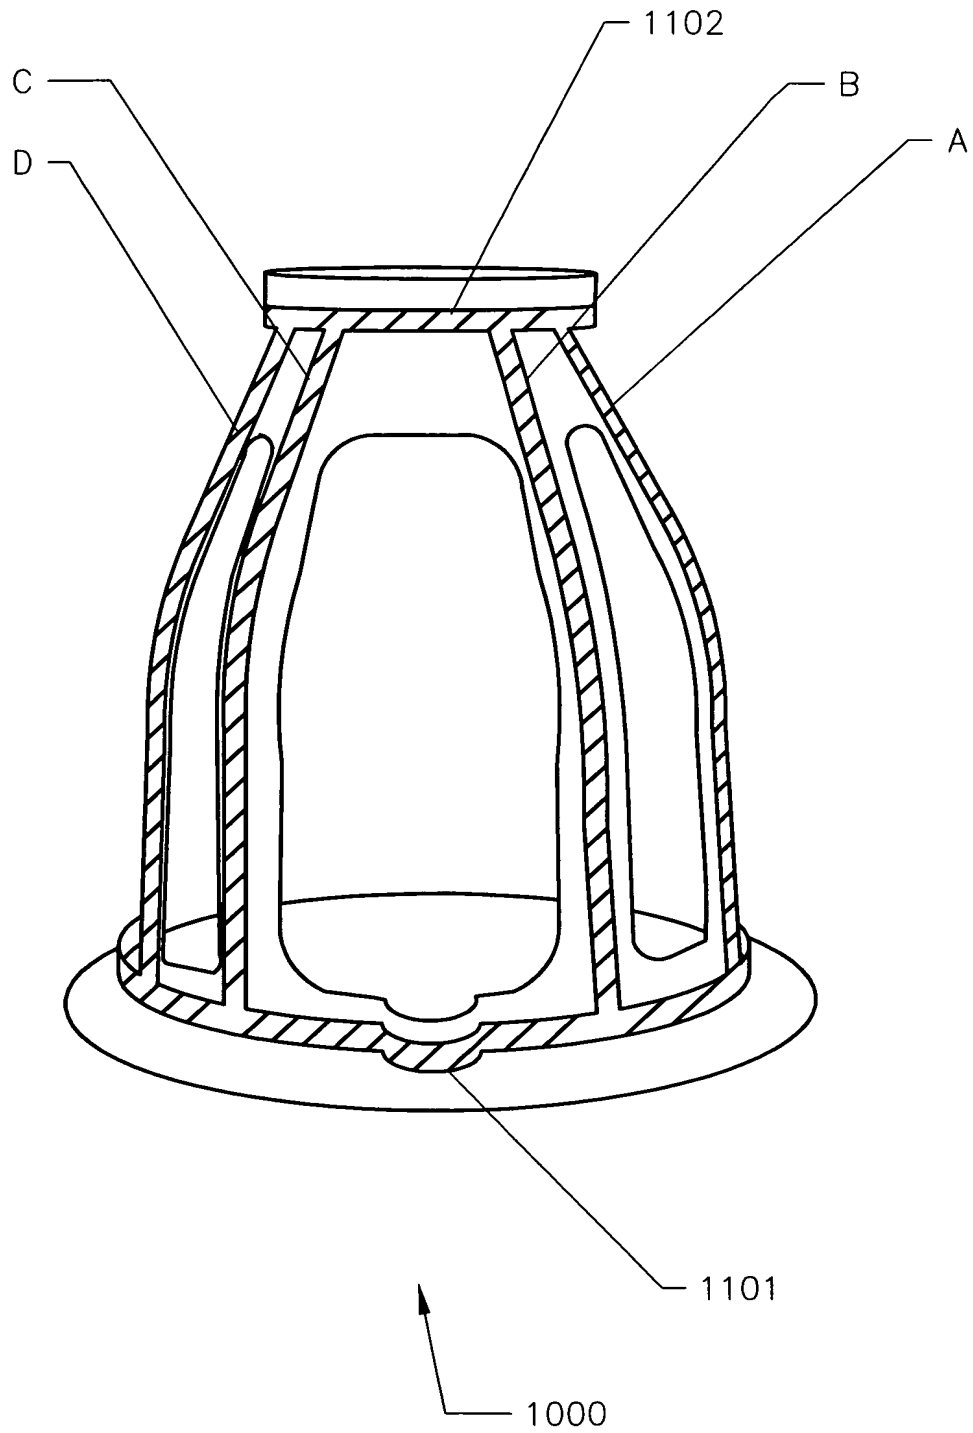


FIG. 3

7/25

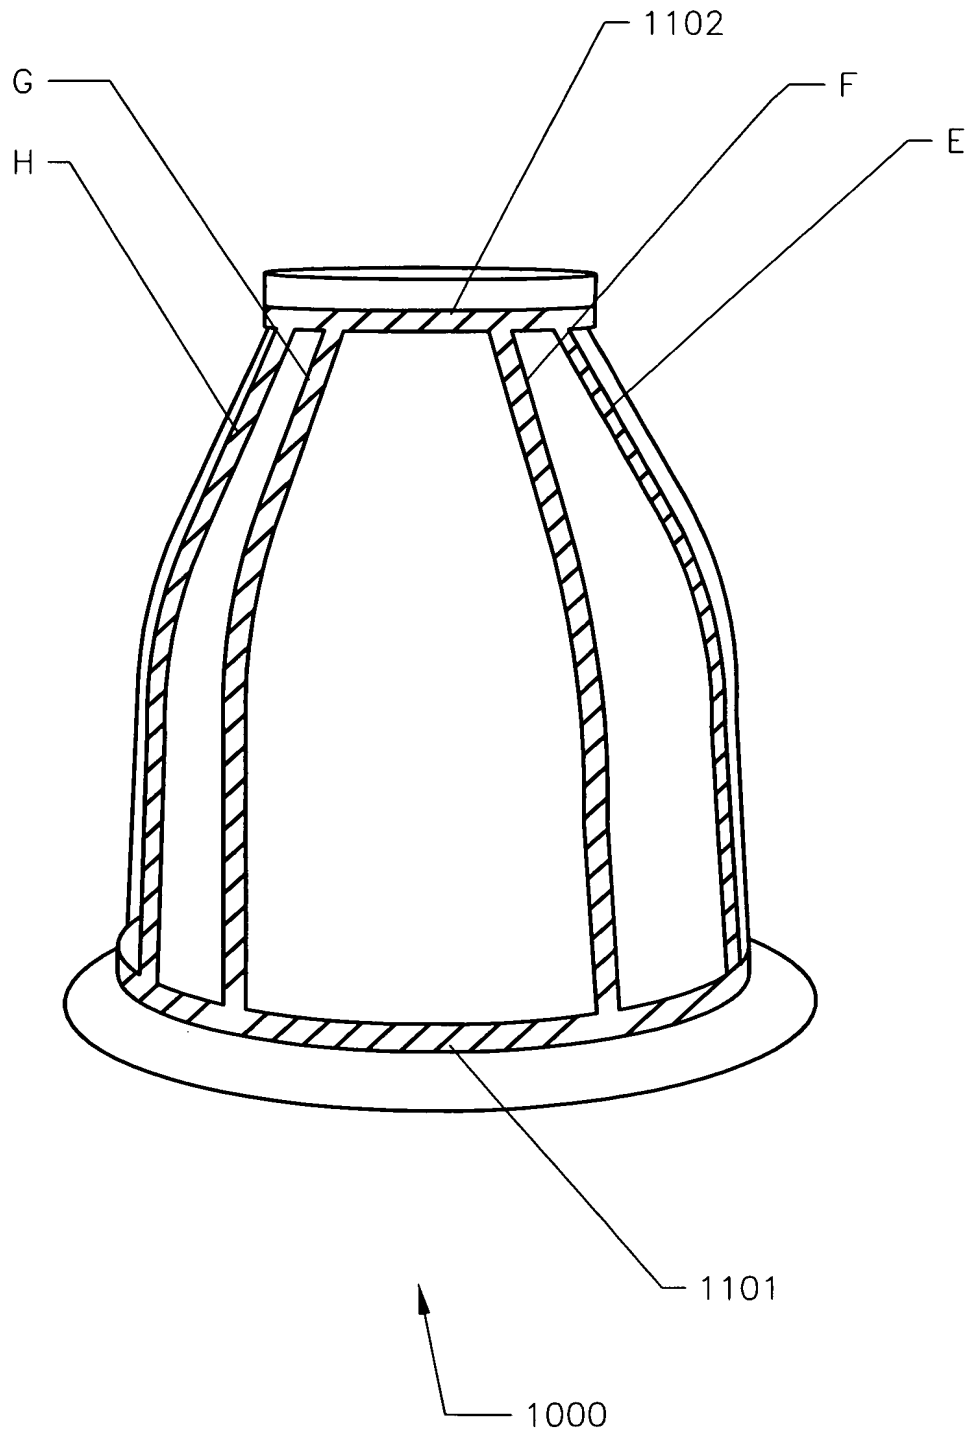


FIG. 4

8/25

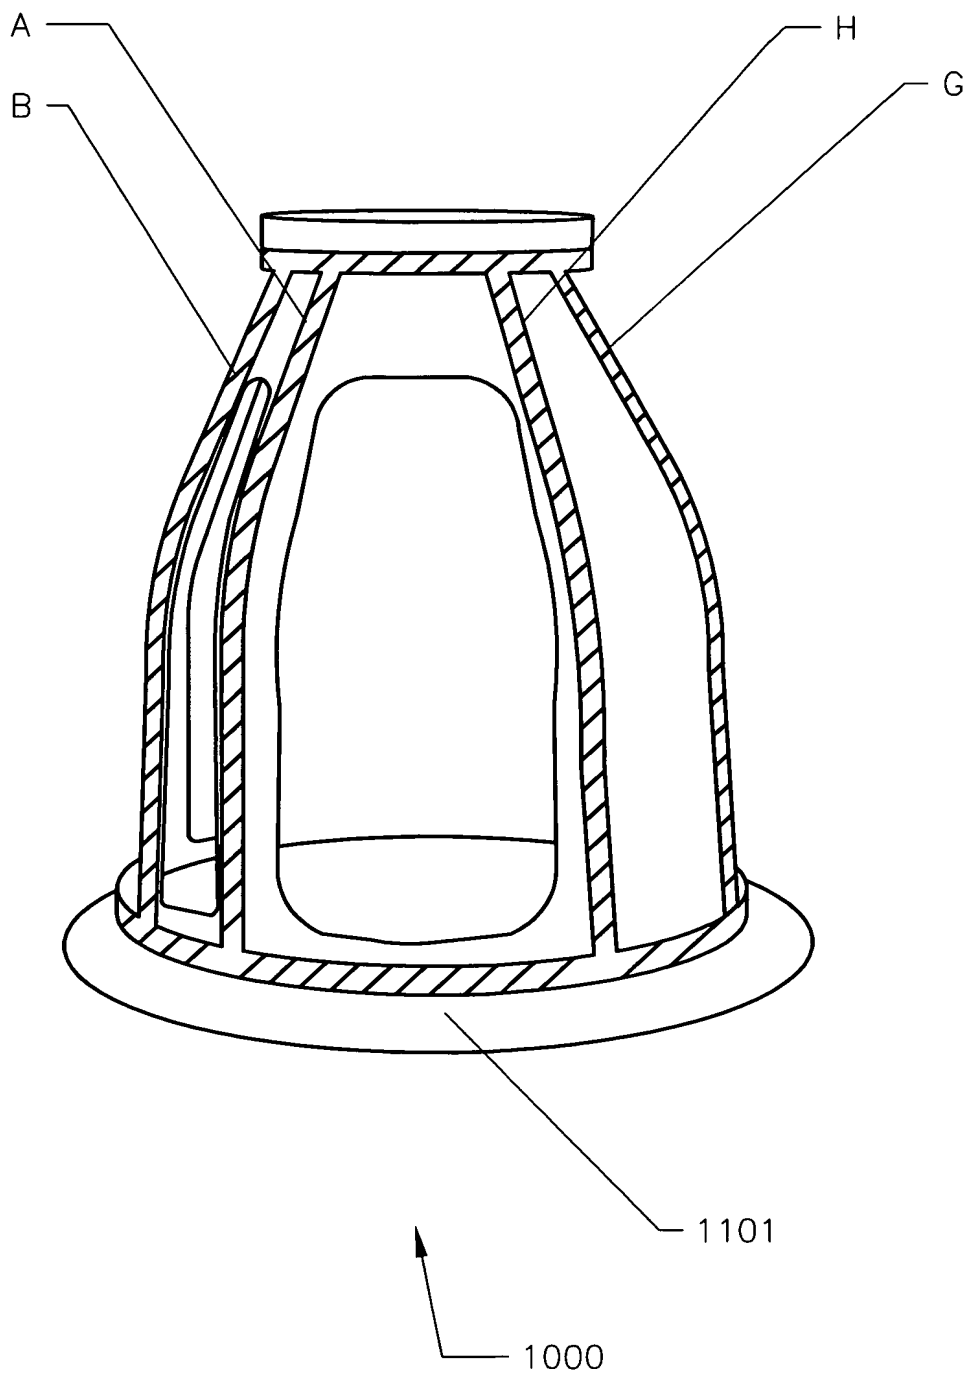


FIG. 5

9/25

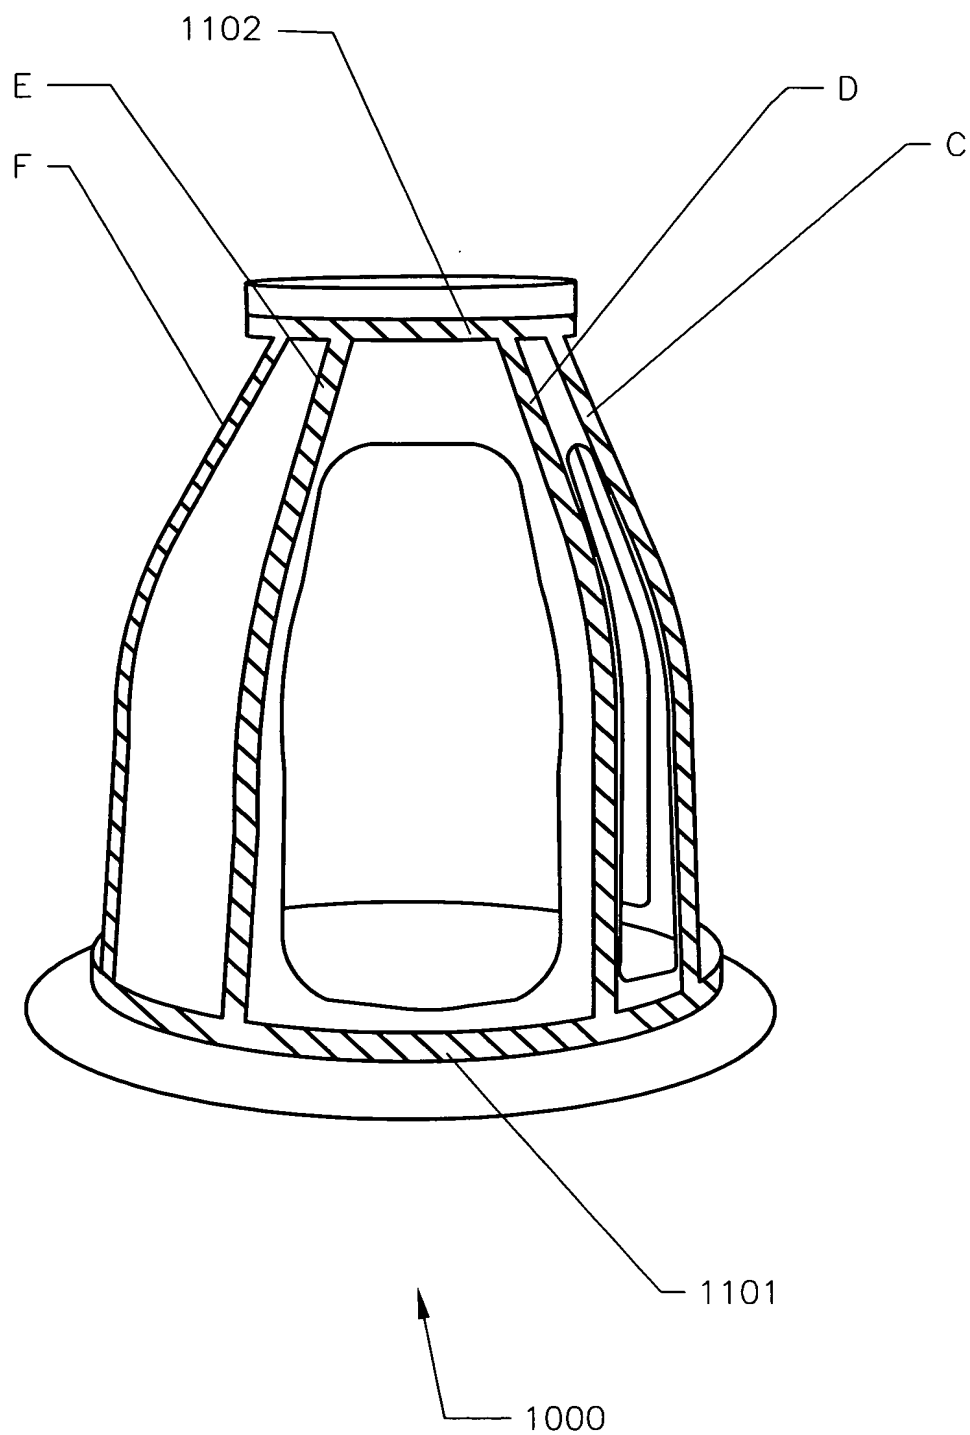


FIG. 6

10/25



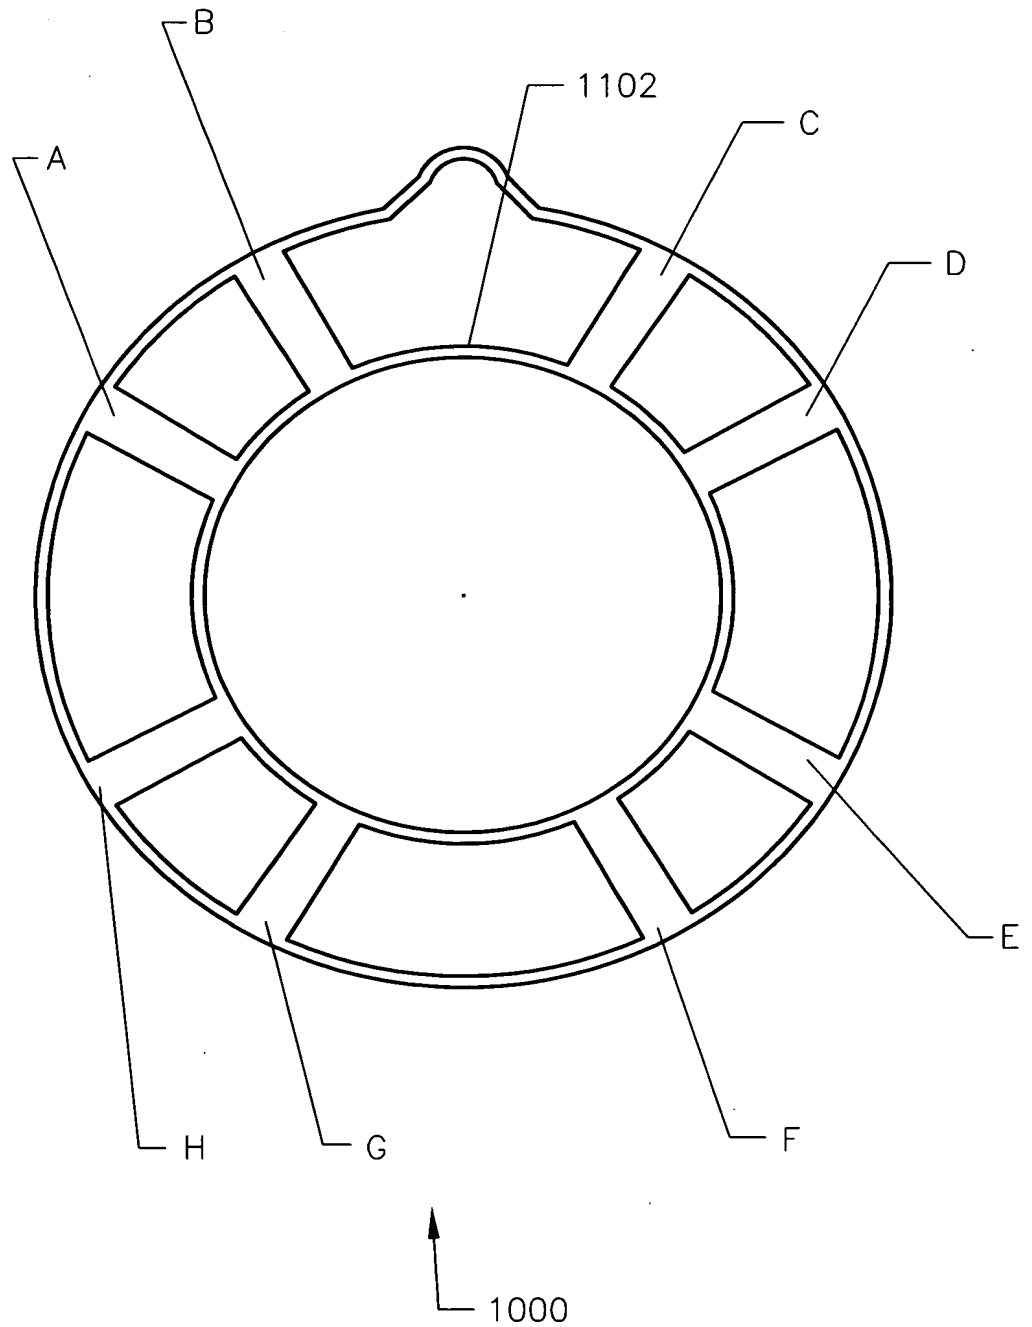


FIG. 7

11/25


$$\frac{F}{G} \infty$$

12/25

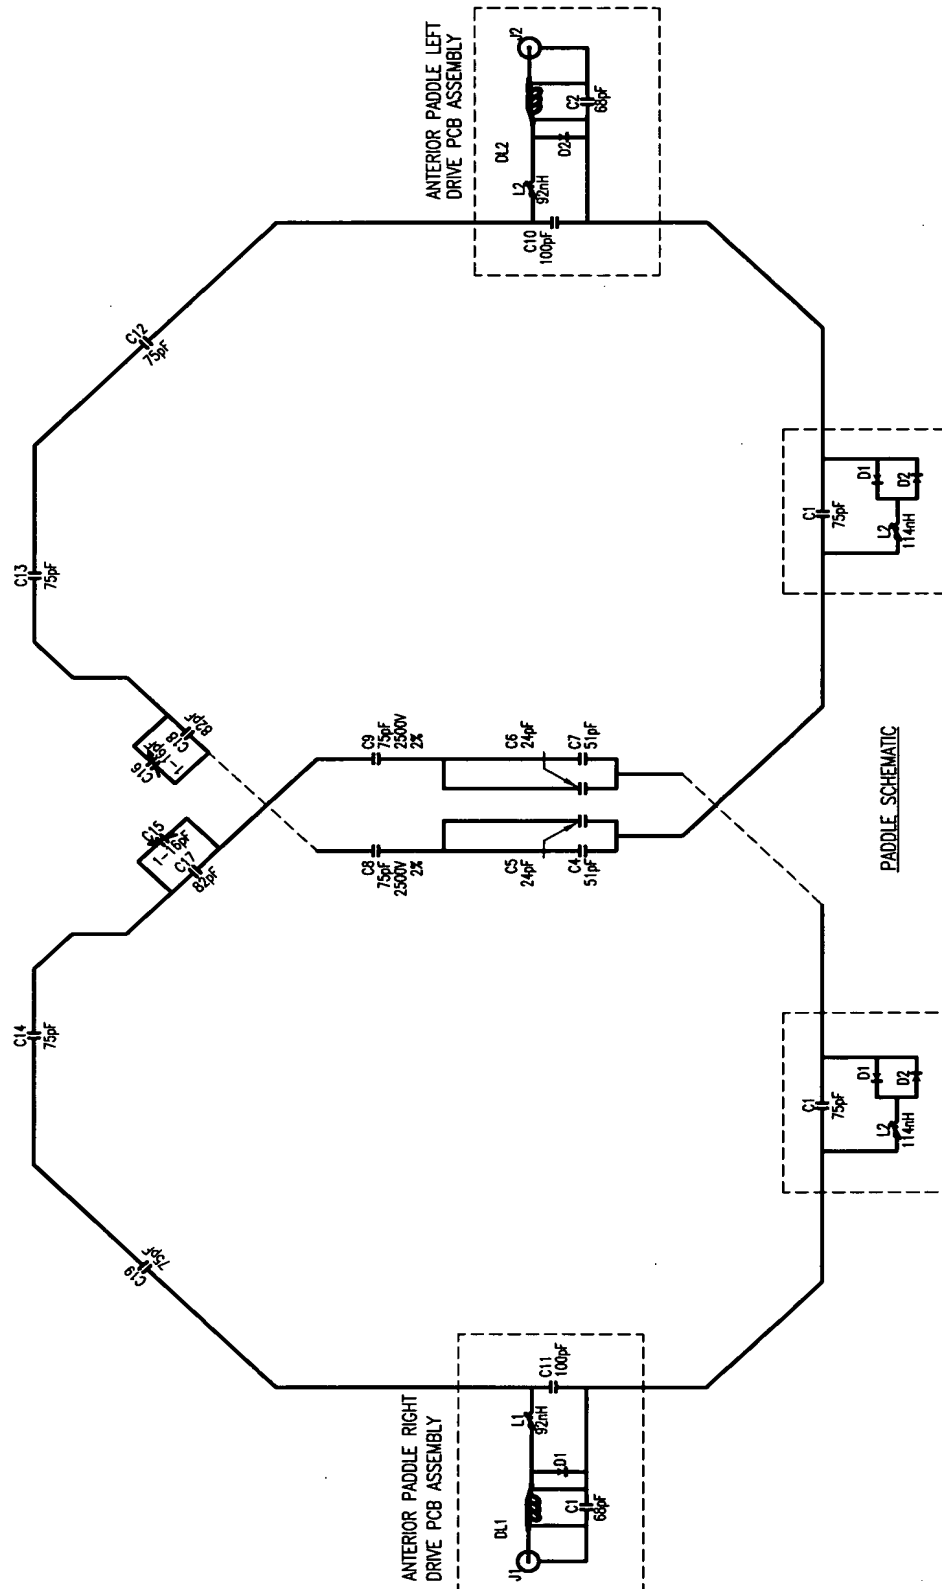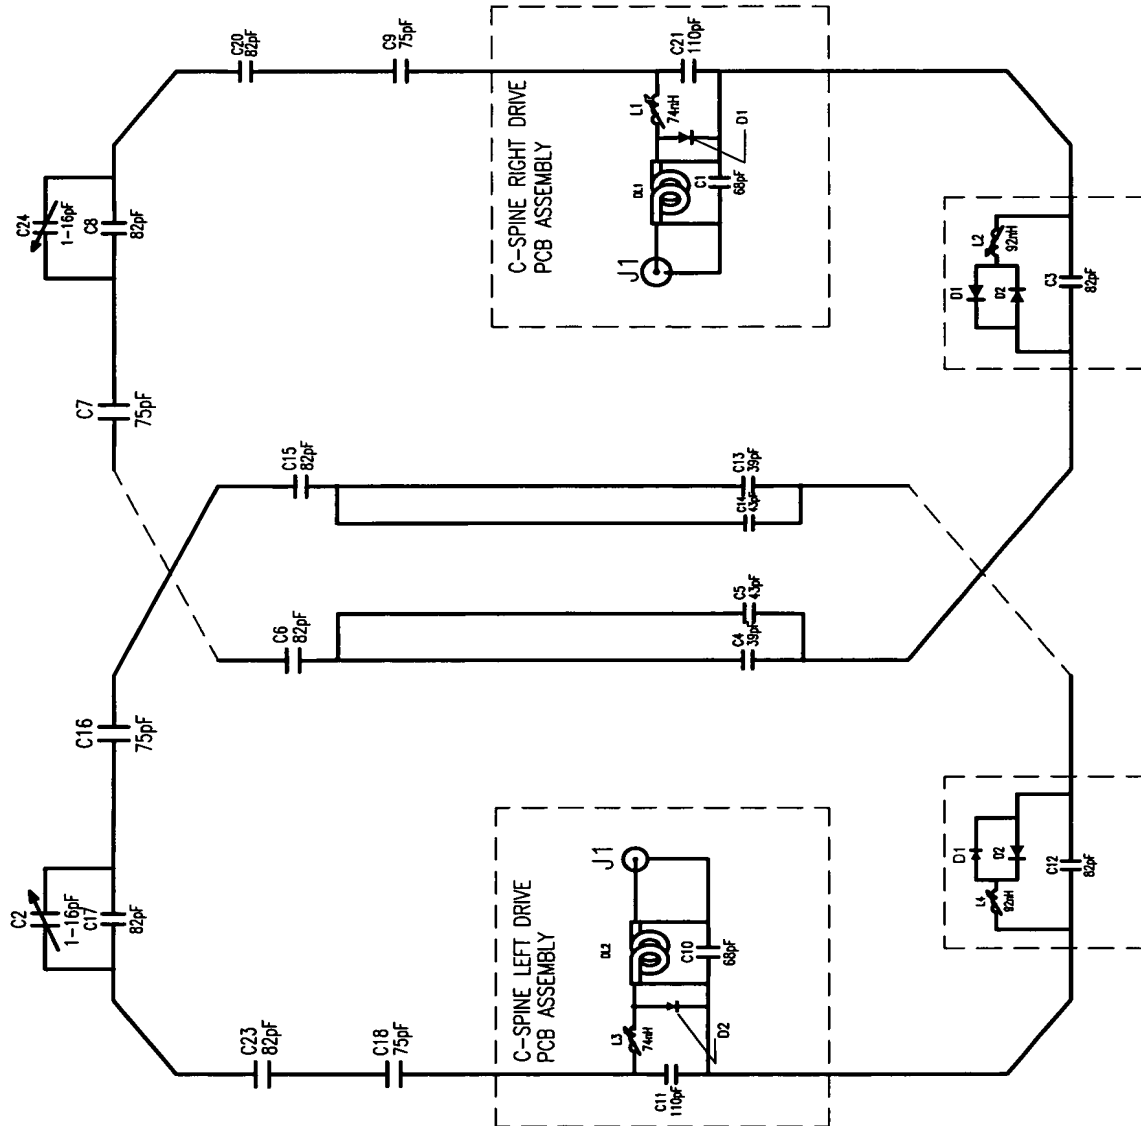

13/25

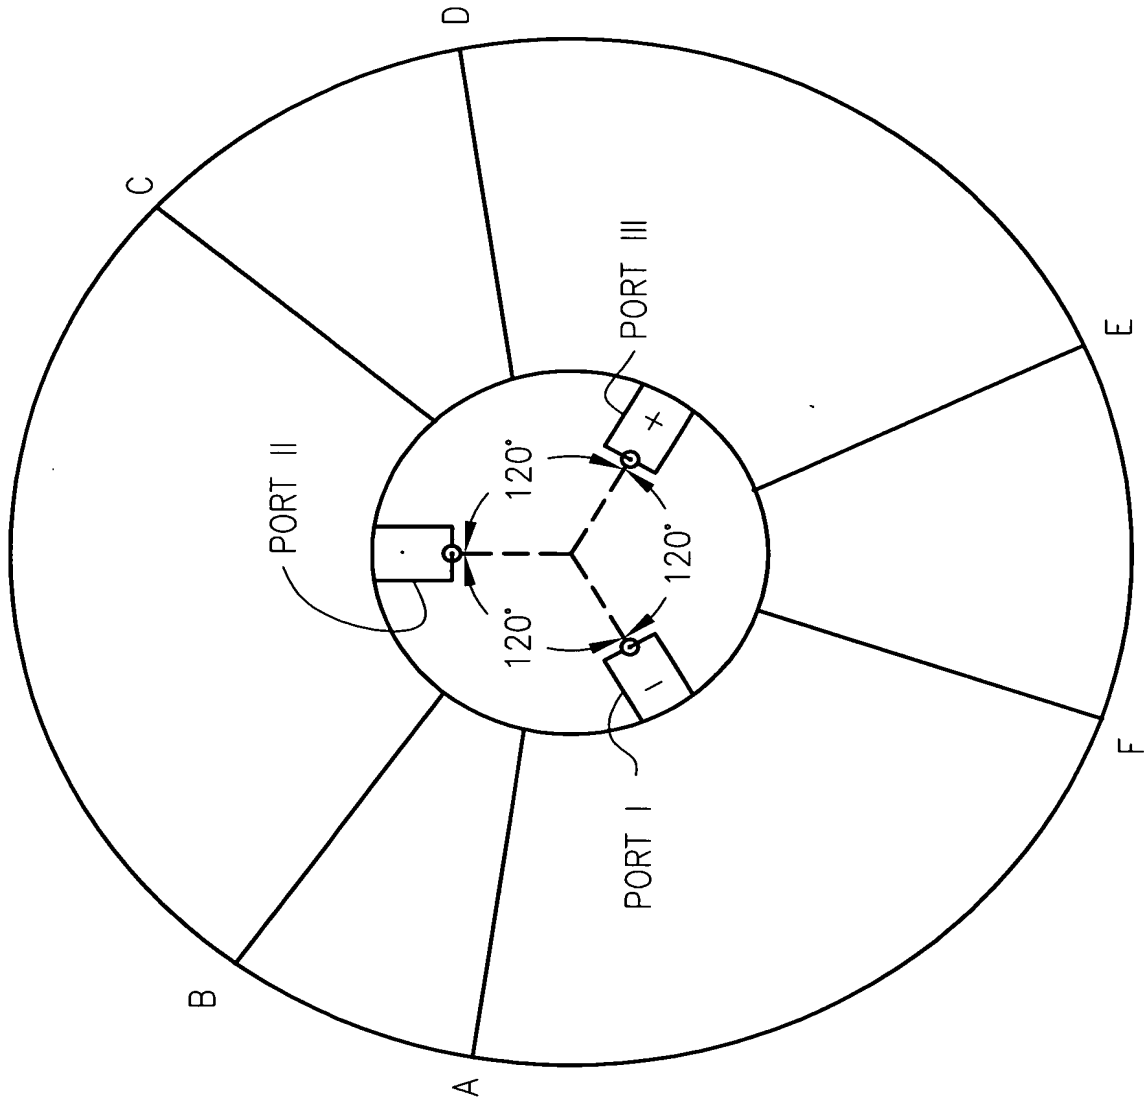


FIG. 10

14/25

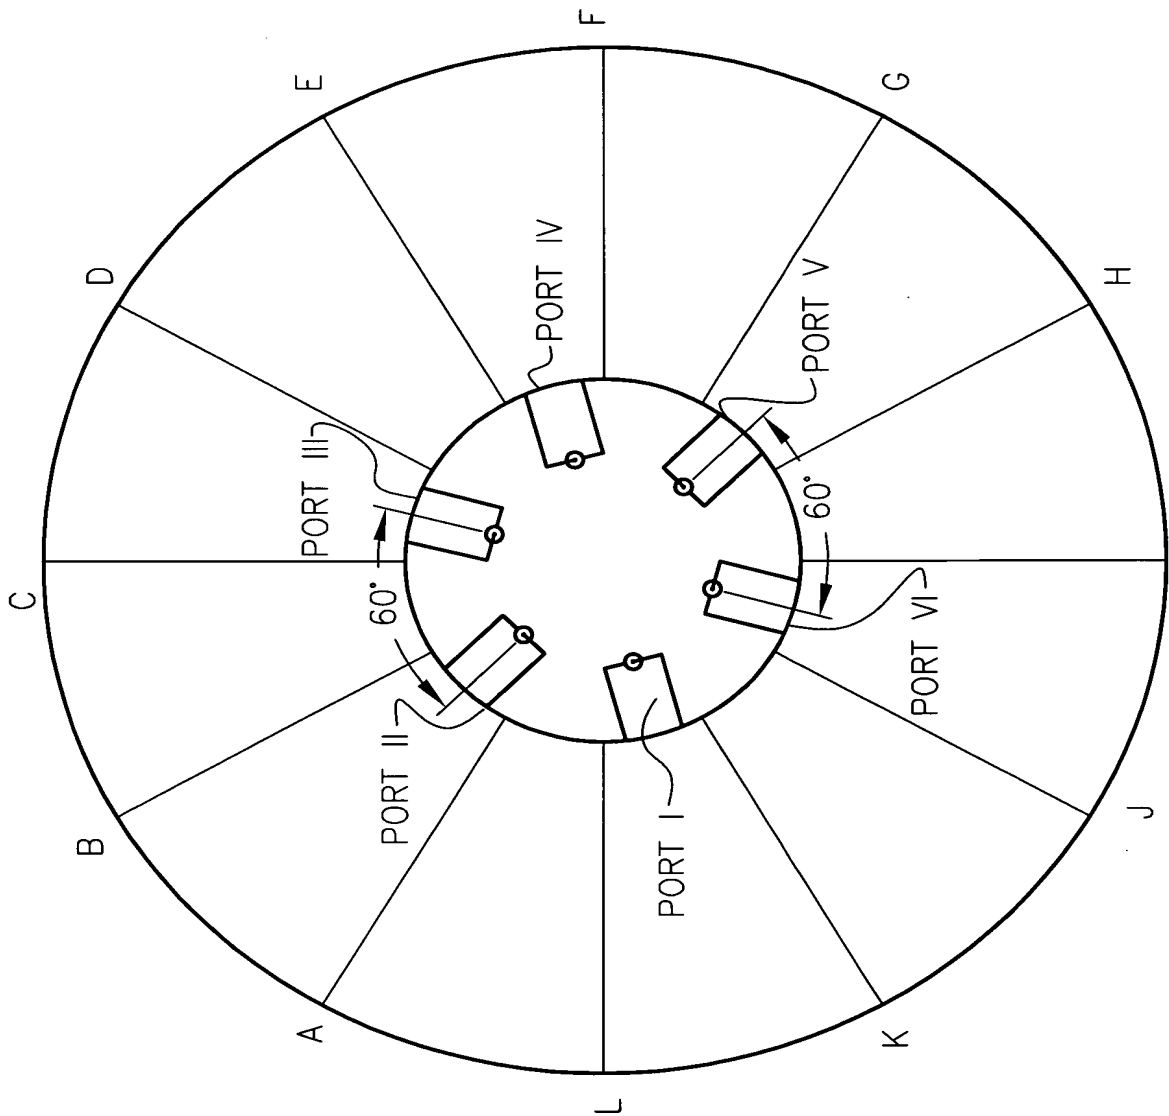


FIG. 11

15/25

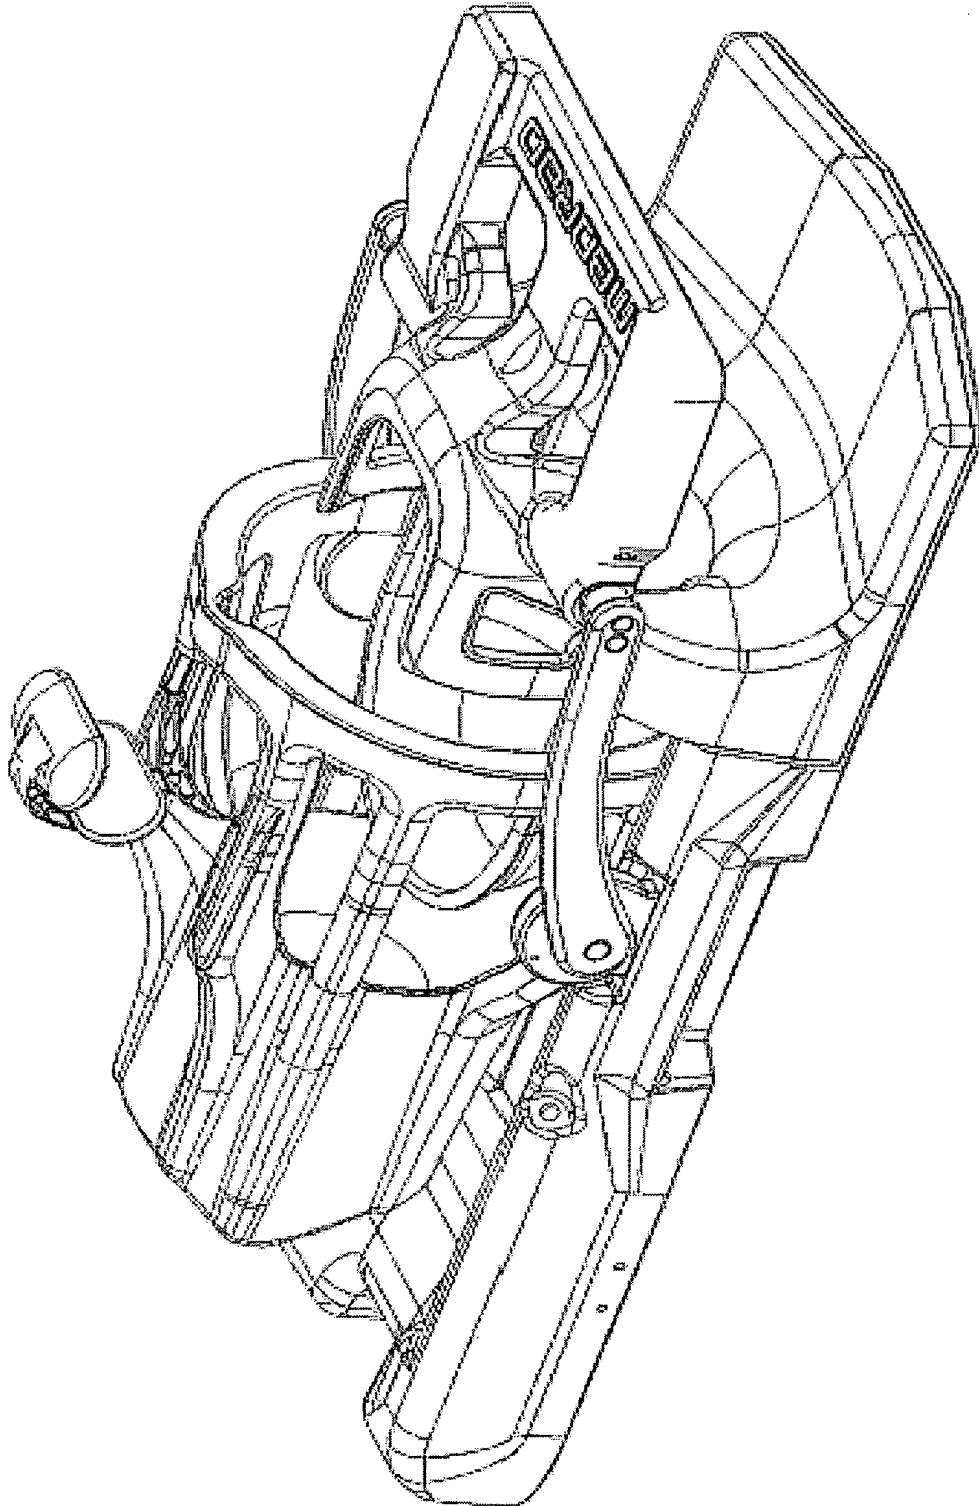


FIG. 12

16/25

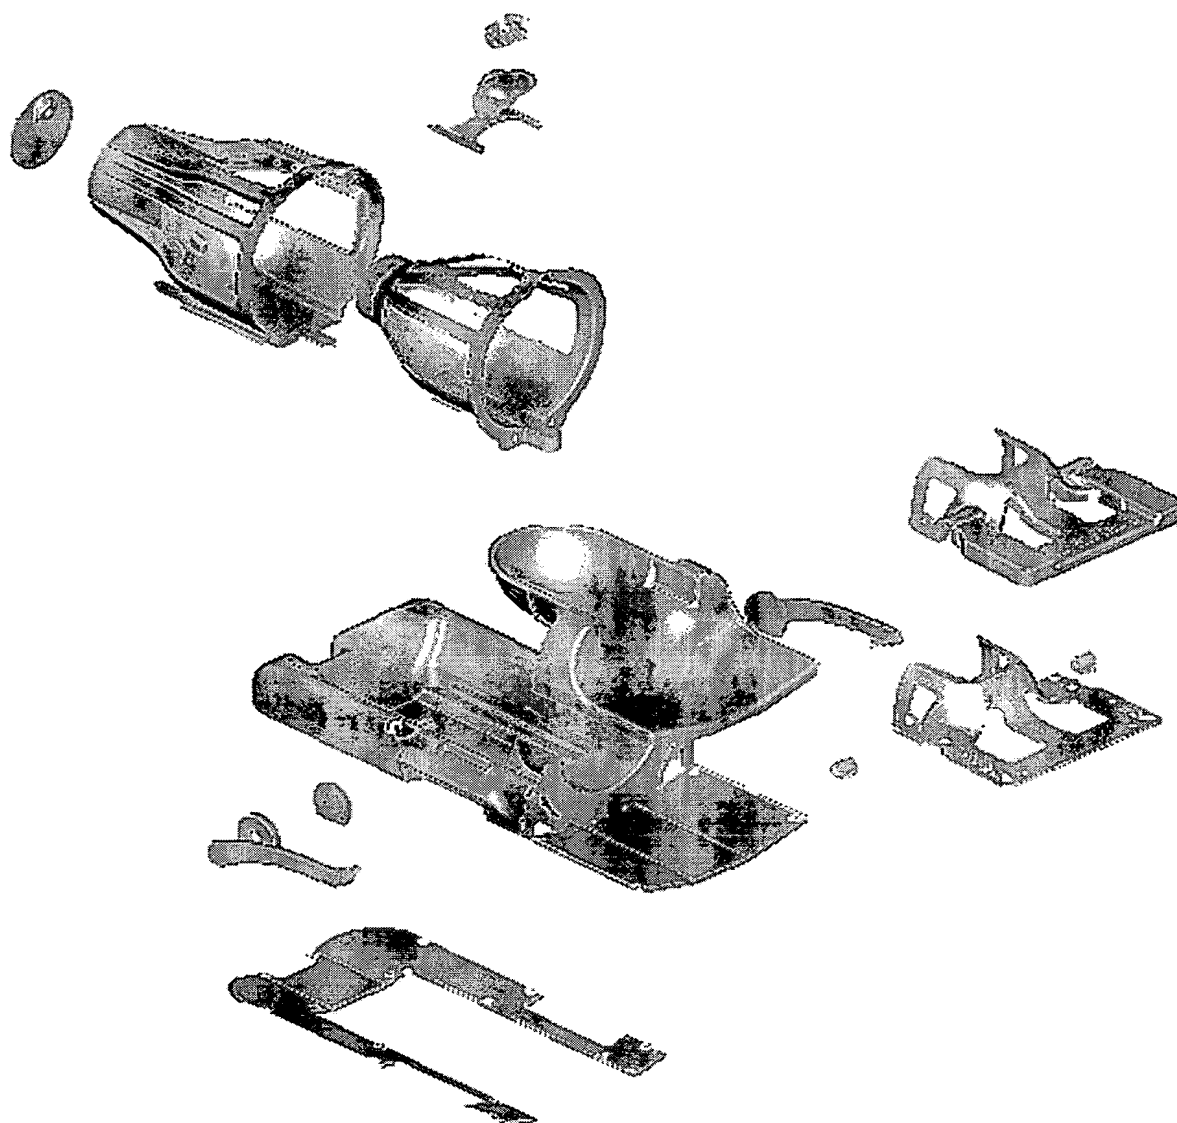


FIG. 13

17/25

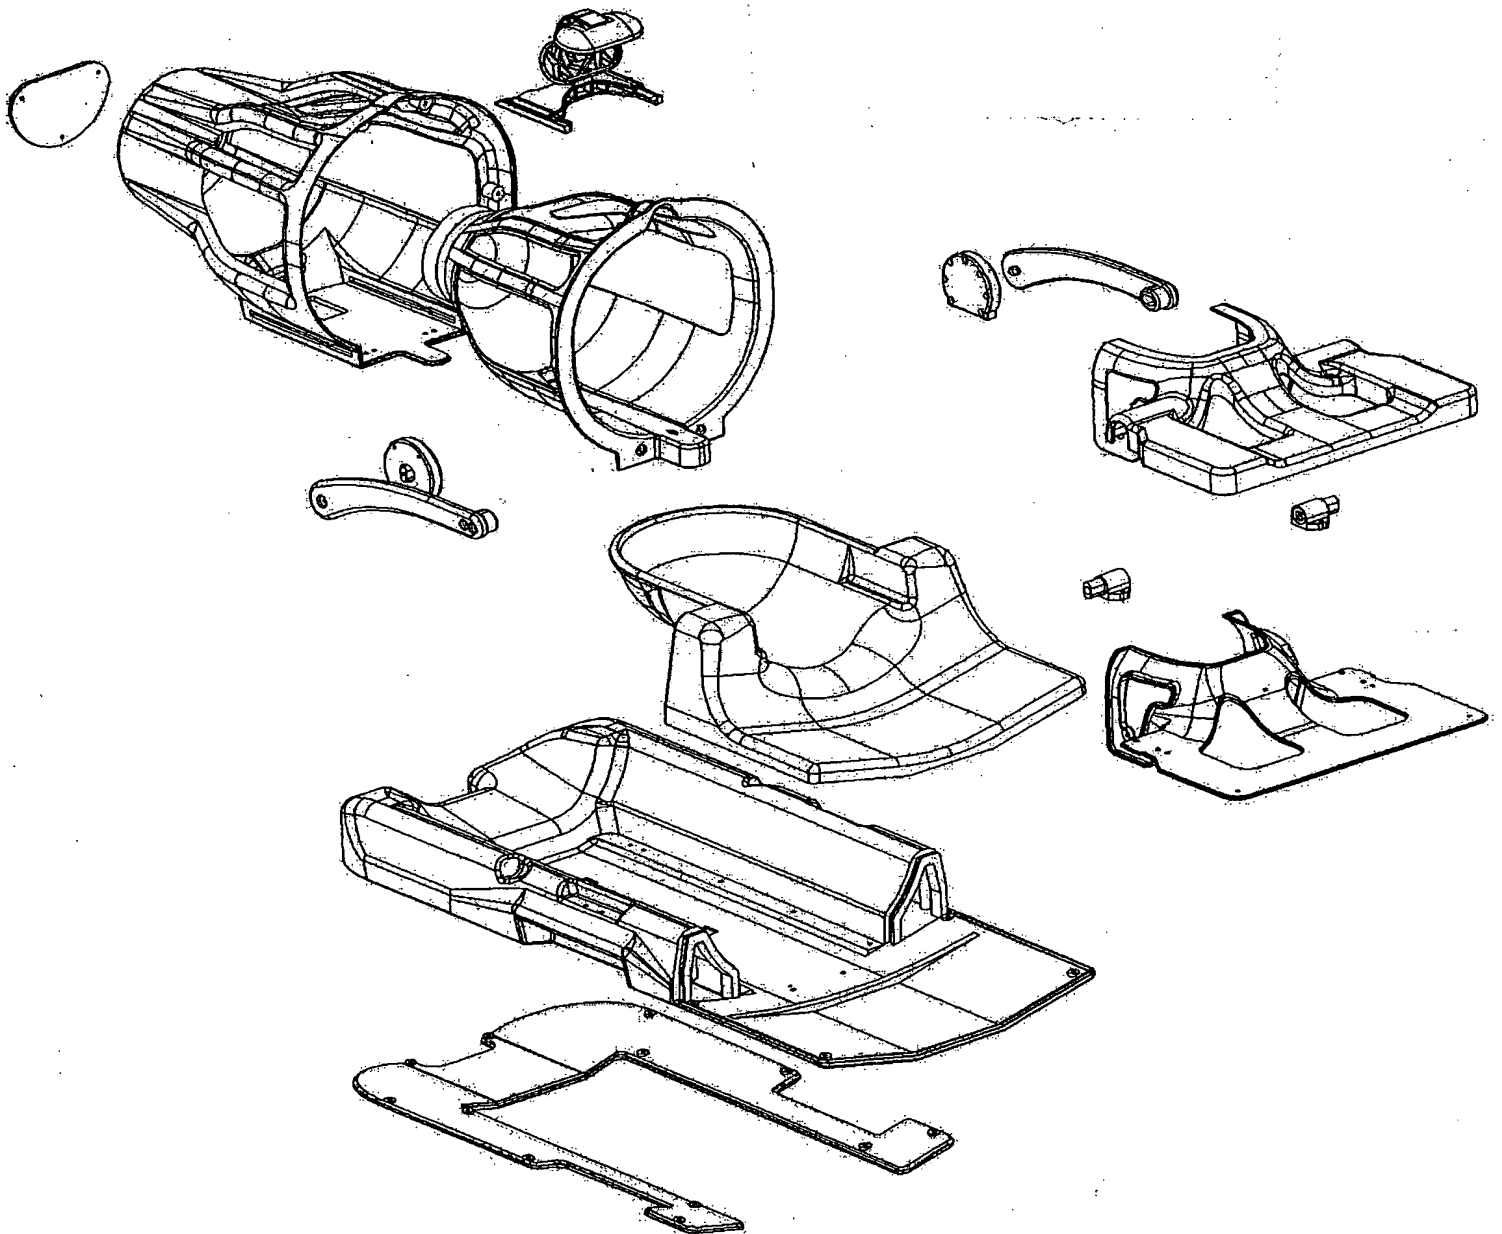


FIG. 14

18/25

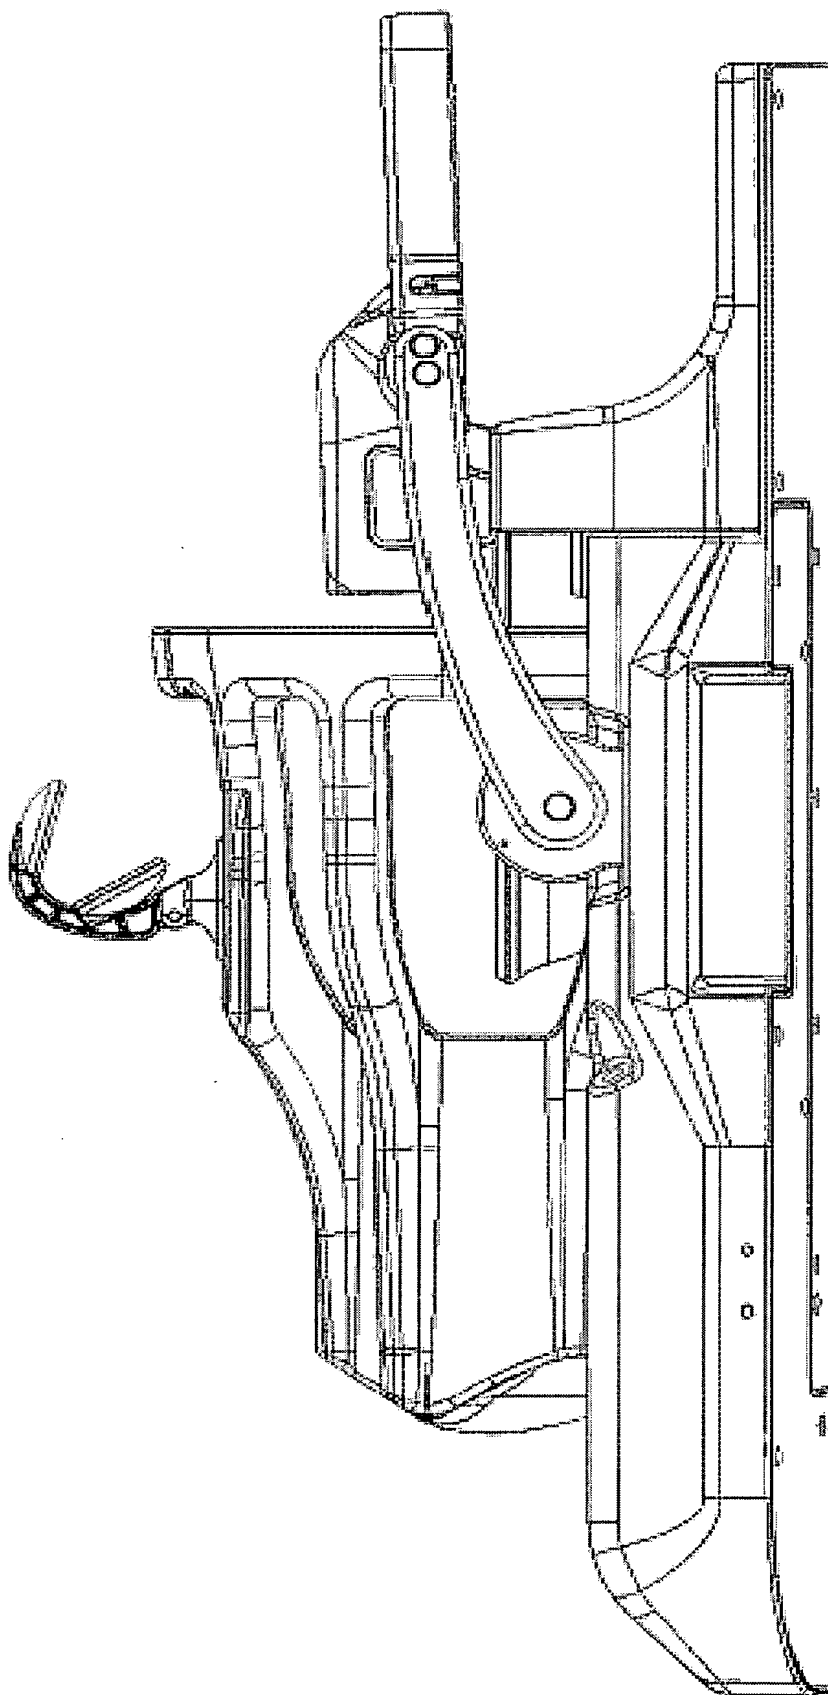


FIG. 15

19/25

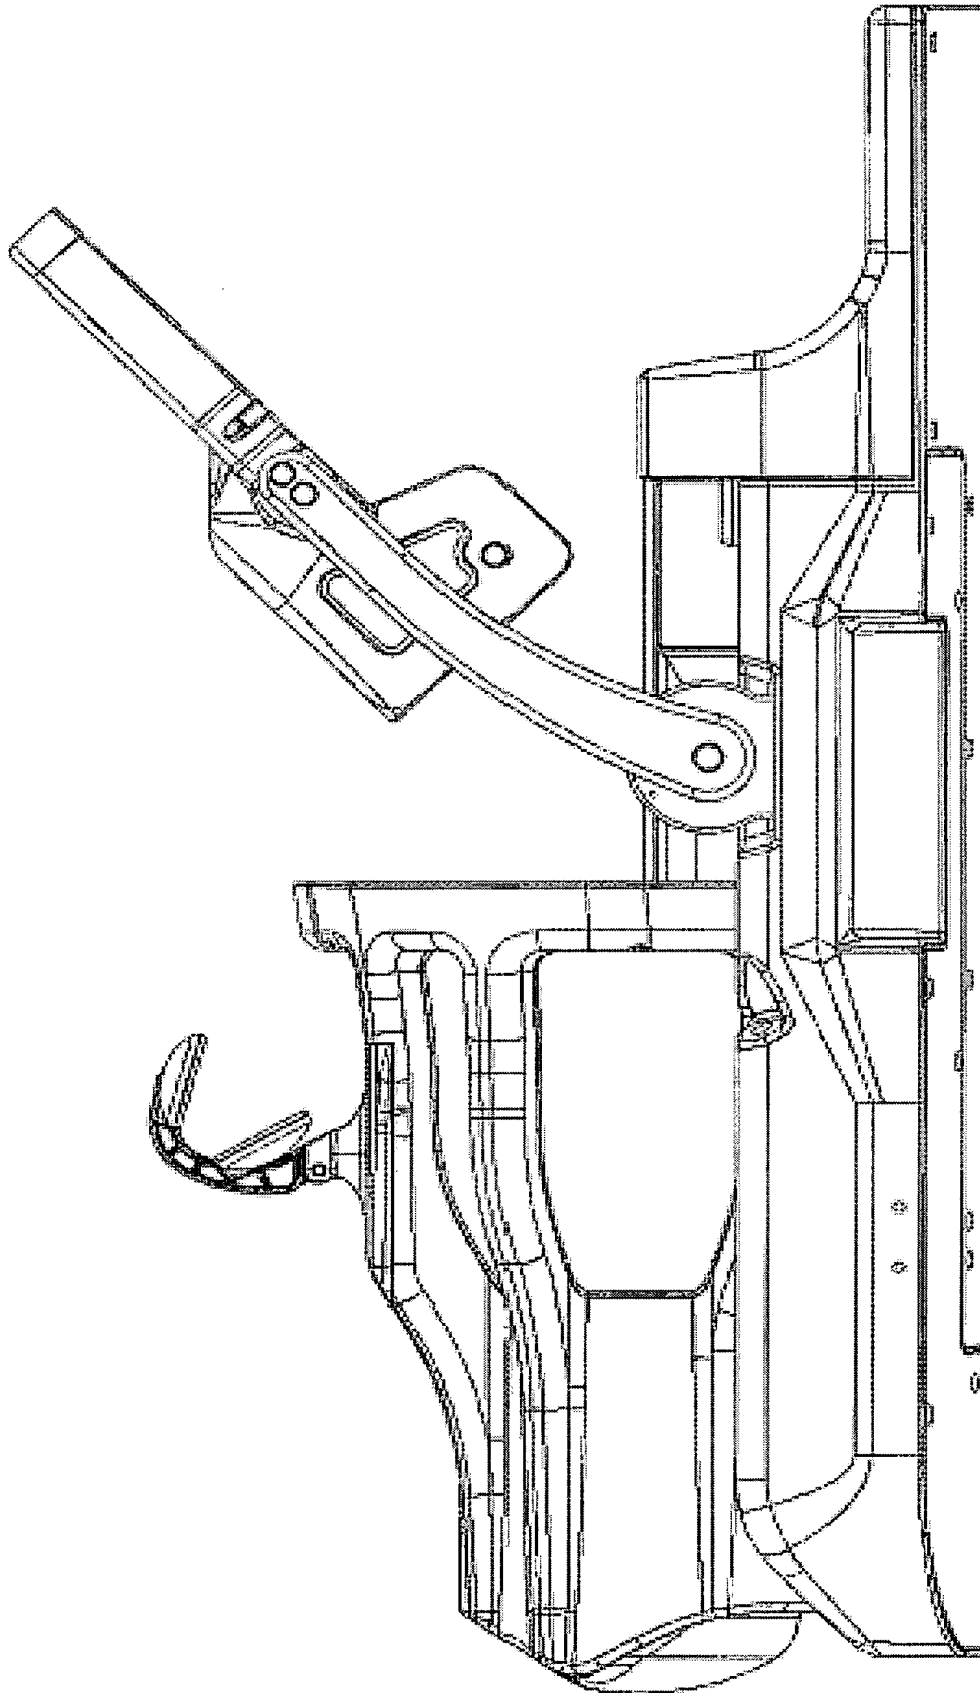


FIG. 16

20/25

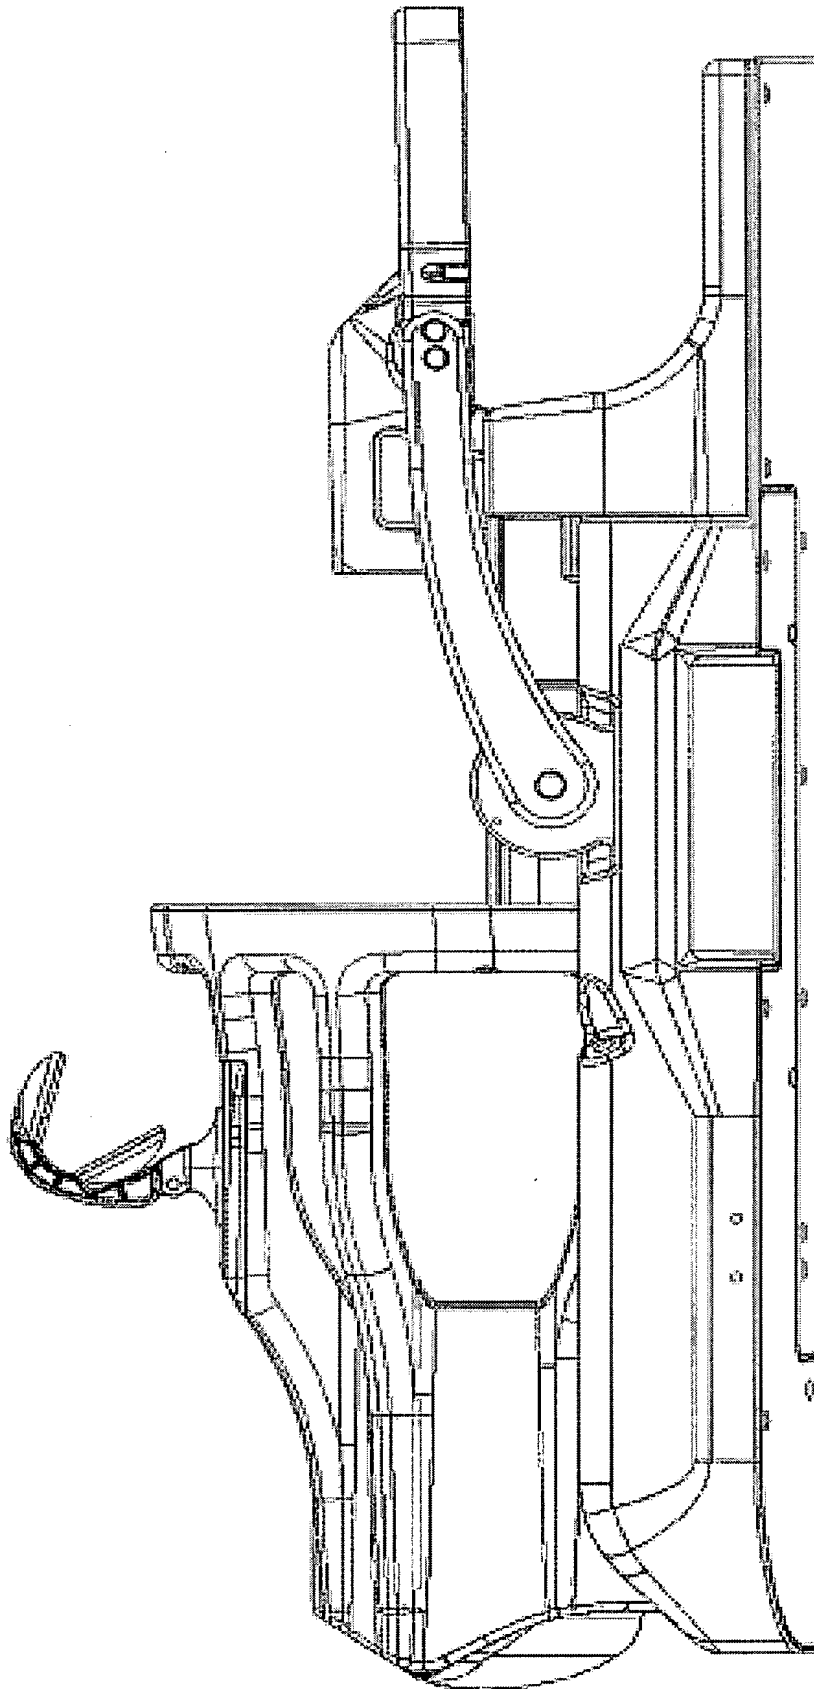


FIG. 17

21/25

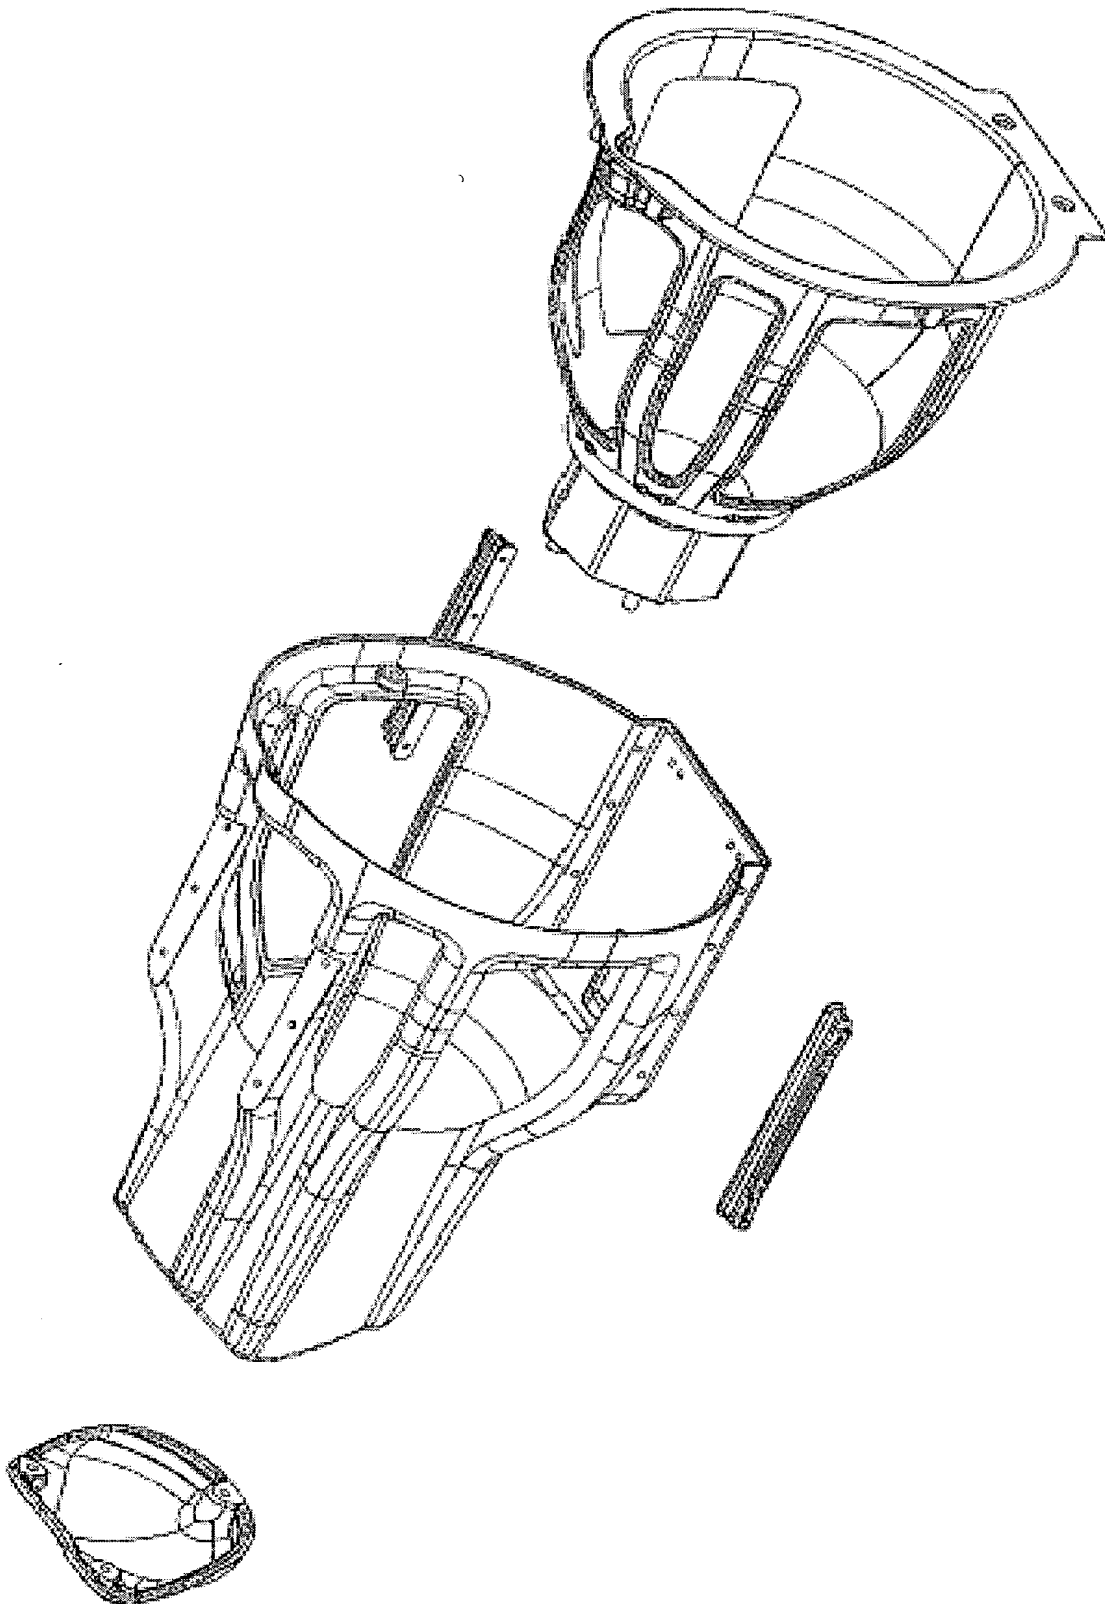


FIG. 18

22/25

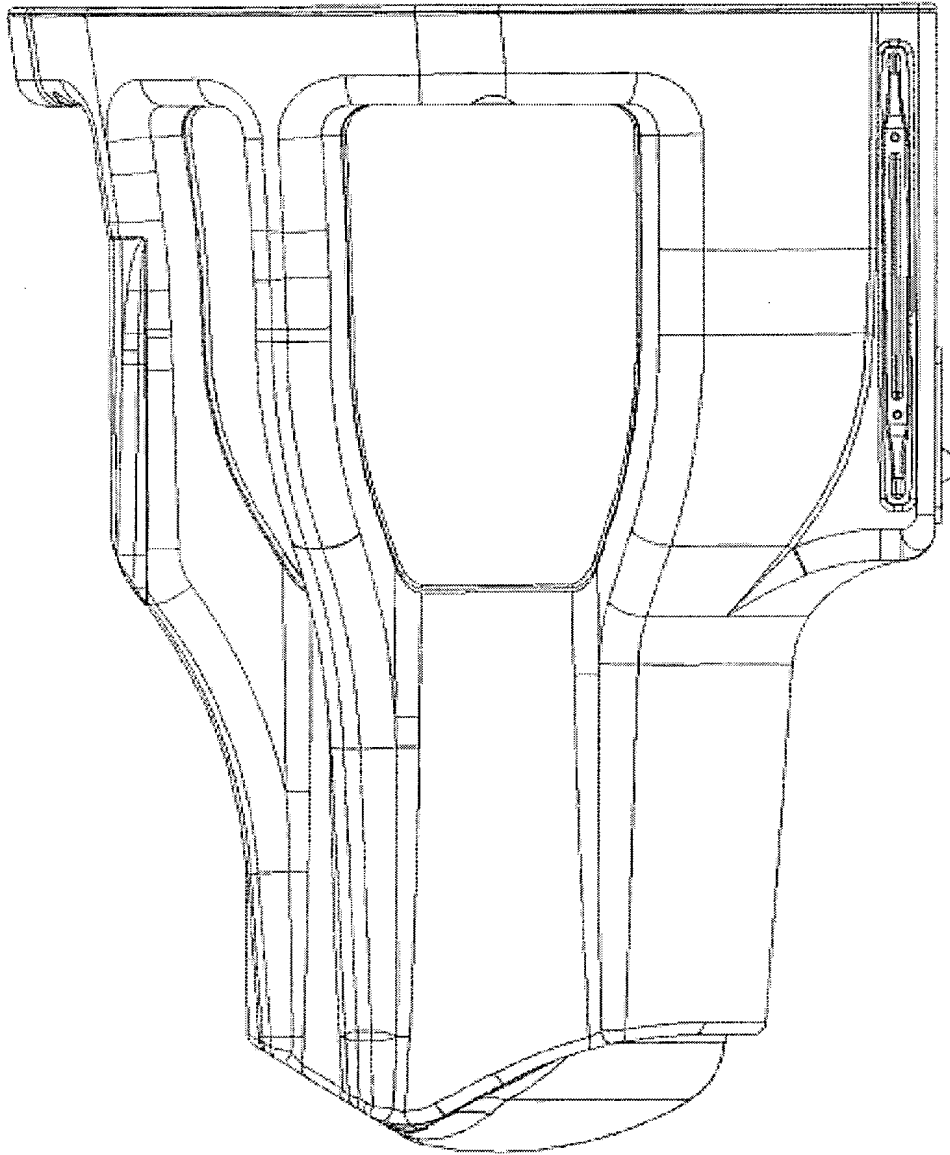


FIG. 19

23/25

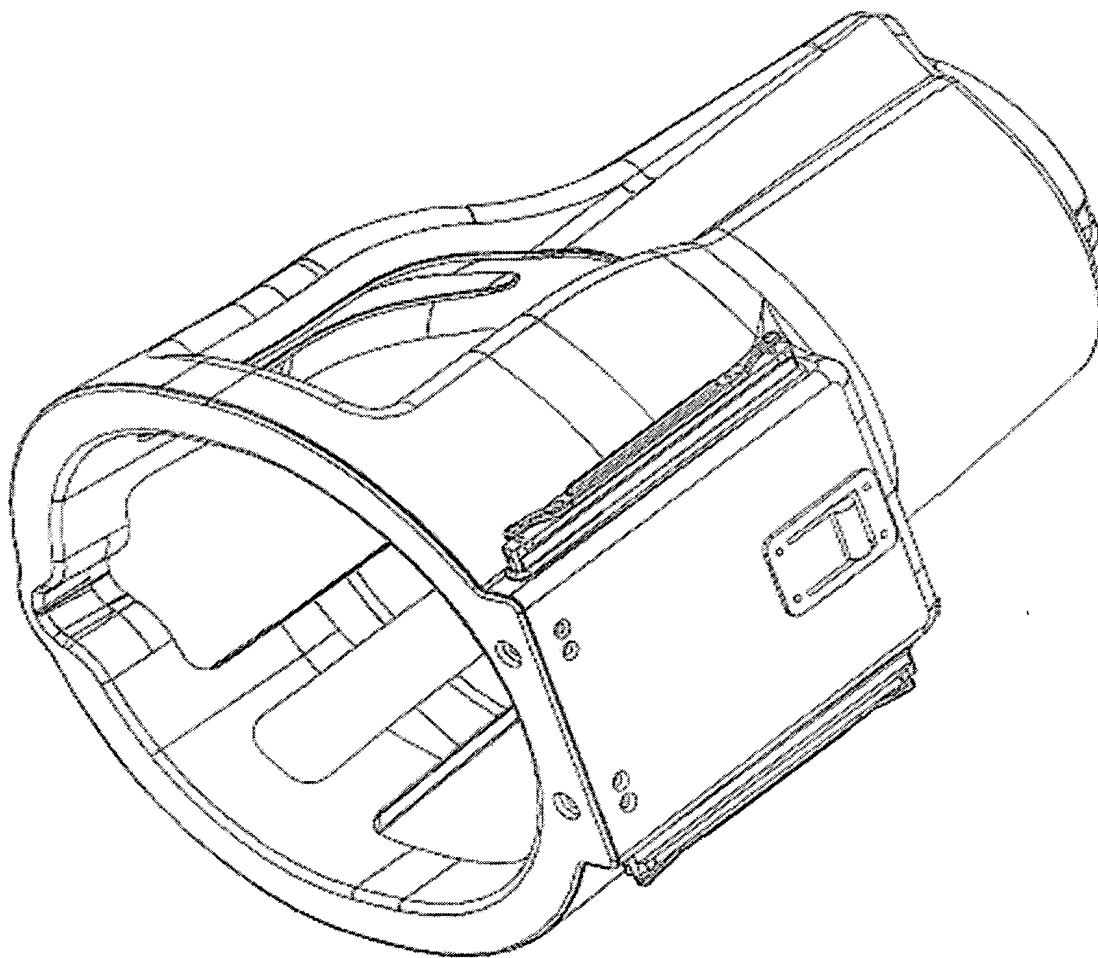


FIG. 20

24/25

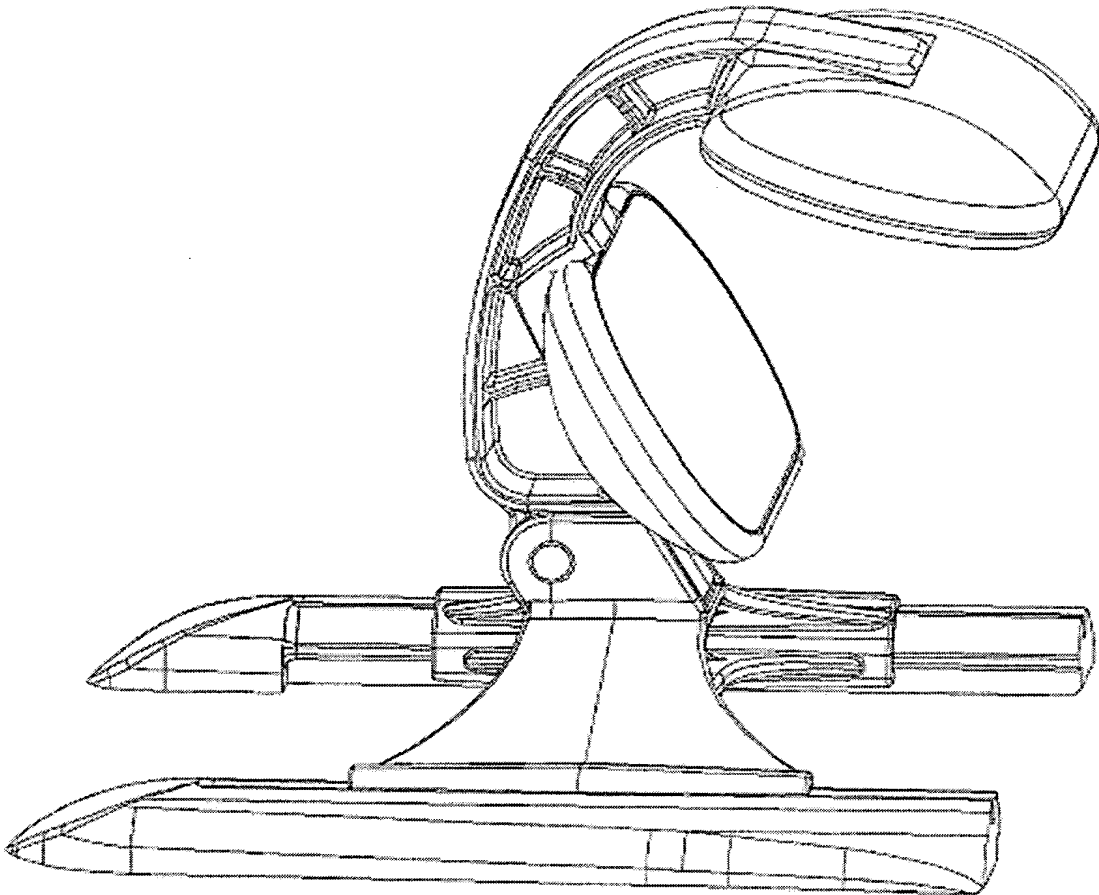


FIG. 21

25/25

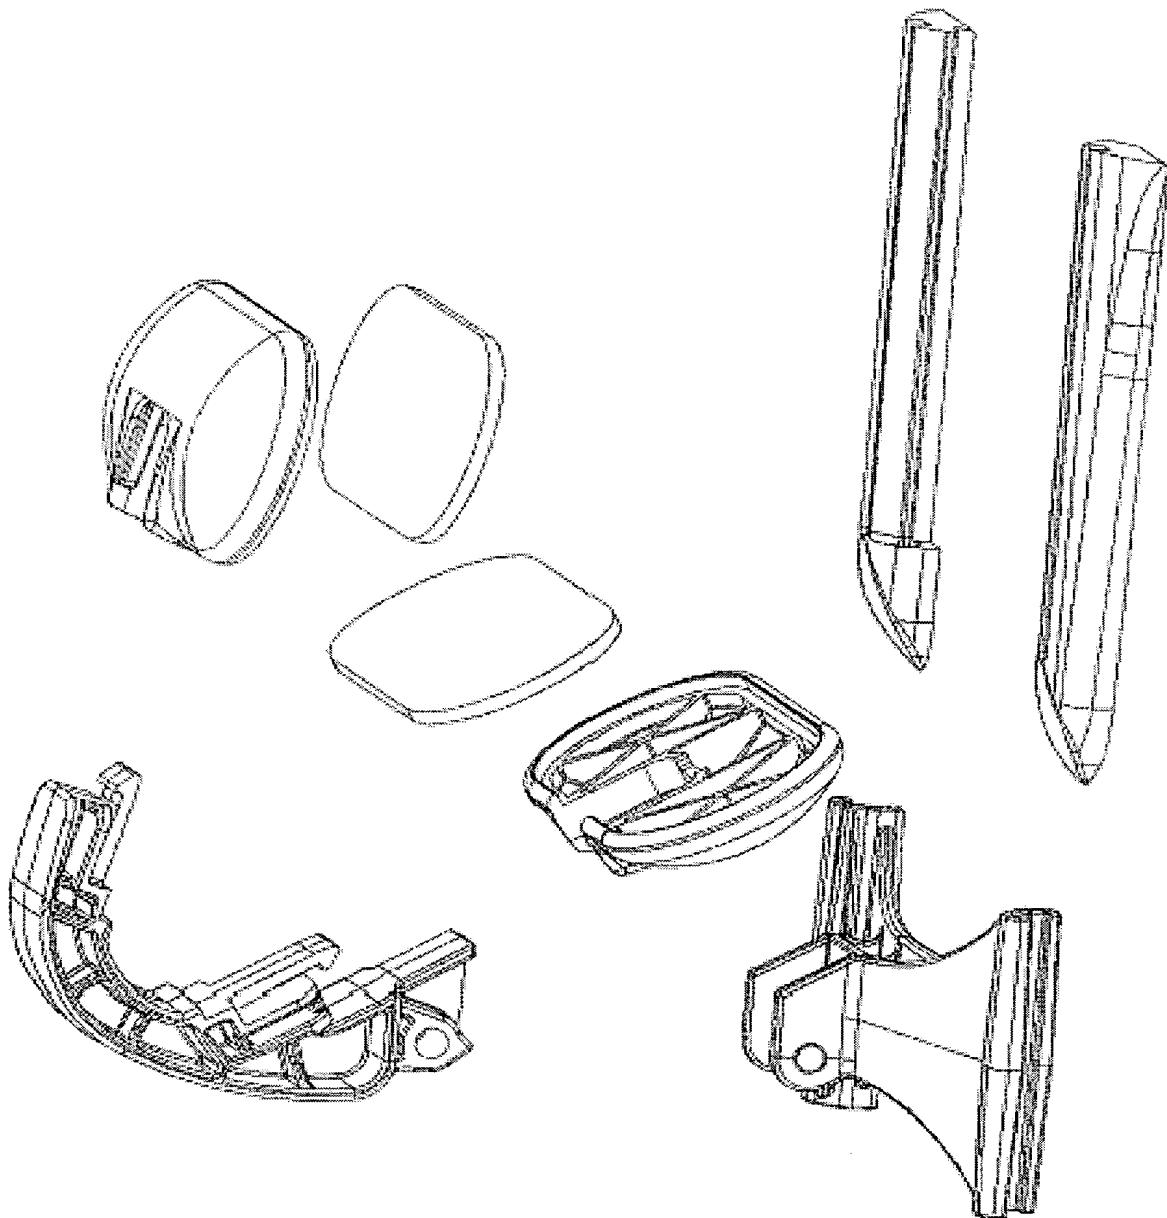


FIG. 22